Pediatric Nailing Platform FEMUR

SURGICAL TECHNIQUE



OrthoPediatrics®
Leading Innovation in Pediatric Orthopedics

Acknowledgements

Emory Chang, MD
Pediatric Orthopedic Surgery
Miller Children's and Women's Hospital
Long Beach, CA
USA

Eric Gordon, MD
Professor
Pediatric Orthopedic Surgery
Washington University in St. Louis School of Medicine
St. Louis, MO
USA

Mark Seeley, MD
Associate Professor
Pediatric Orthopedic Surgery
Geisinger Commonwealth School of Medicine
Danville, PA
USA

Peter Stevens, MD
Professor
Pediatric Orthopedic Surgery
University of Utah
Salt Lake City, UT
USA

Ira Zaltz, MD
Professor
Pediatric Orthopedic Surgery
Oakland University William Beaumont School of Medicine
Royal Oak, MI
USA

TABLE OF

Contents

System Overview

System Features 4
Indication 6
Preoperative Planning 7
Nail Size Selection 7
Entry Point and Entry Angle 8

Surgical Technique

Patient Positioning 9
Approach 10
Measuring 16
Reaming Technique. 18
Targeting Guide Nail. 20
Nail Placement 21
Proximal Interlocking 25
Distal Interlocking. 28
Closure & Post-Operative Care 30
Nail Removal 31

Product Information

Screw Driver Options 33
Explantation Driver 34
CHILD Nails. 35
ADOLESCENT Nails. 37
End Caps 39
Screws 40
Instruments 41
Important Medical Information 44

SYSTEM FEATURES

	CHILD Nails		
	7mm	8mm	9mm
Nails			
Material	316L Stainless Steel		
Head Diameter	9mm		
Shaft Diameter	7mm	8mm	9mm
Lengths, 2cm Increments	20-38cm	24-42cm	28-42cm
Proximal Bend	10°		
Radius of Curvature	1.45m		
Attachment Bolt	¼" - 28		
Guide Wire Exchange	Yes		
Proximal Locking			
Descending Oblique Screw	Yes		
Transverse Screw	Yes		
Recon Screw	Yes--one screw @ 135° NSA		
Anteversion	14°		
Screw Diameter	4.5mm Fully Threaded		
	4.5mm Partially Threaded		
Distal Locking			
Lateral-Medial Static	Yes		
Lateral-Medial Dynamic	Yes--5mm dynamization		
Anterior-Posterior Static	Yes		
Screw Diameter	3.8mm/4.0mm	4.5mm	
All Screws			
Material	316L Stainless Steel		
Hex Size	3.5mm		
Head Diameter	6.5mm		
End Caps			
Material	316L Stainless Steel		
Hex Size	3/16"		
Head Diameter	9mm, except Flush size		
Lengths	Flush, +5, +10, +15, +20		

NOTE: The 3.8mm unicortical peg and 4.0 fully threaded screw are only used for distal locking of the 7mm nail.



CHILD Left Nails: 7mm x 28cm, 8mm x 32cm,9mm x 36cm shown (left to right).



ADOLESCENT Right Nails: 9mm x 30cm, 10mm x 34cm, 11mm x 38cm, 12mm x 42cm shown (right to left).

ADOLESCENT Nails				
9mm	10mm	11mm	12mm	
Nails				
316L Stainless Steel				Material
10mm		11mm	12mm	Head Diameter
9mm	10mm	11mm	12mm	Shaft Diameter
28-48cm*	30-48*cm			Lengths, 2cm Increments
10°				Proximal Bend
1.45m				Radius of Curvature
5/16” - 24				Attachment Bolt
No				Guide Wire Exchange
Proximal Locking				
Yes				Descending Oblique Screw
Yes				Transverse Screw
Yes--two screws @ 130° NSA				Recon Screw
14°				Anteversion
5.0mm Fully Threaded				Screw Diameter
5.0mm Partially Threaded				Screw Diameter
Distal Locking				
Yes				Lateral-Medial Static
Yes--5mm dynamization				Lateral-Medial Dynamic
Yes				Anterior-Posterior Static
4.5mm	5.0mm			Screw Diameter
All Screws				
316L Stainless Steel				Material
3.5mm				Hex Size
6.5mm				Head Diameter
End Caps				
316L Stainless Steel				Material
3/16”				Hex Size
10mm, except Flush size				Head Diameter
Flush, +5, +10, +15, +20				Lengths

* 50cm available upon special request

INDICATIONS

The OrthoPediatrics **Pediatric Nailing Platform | Femur** is designed for use in pediatric and small stature adult patients as indicated to stabilize fractures of the femoral shaft; subtrochanteric fractures; ipsilateral neck/shaft fractures; prophylactic nailing of impending pathologic fractures; nonunions and malunions; fixation of femurs that have been surgically prepared (osteotomies) for correction of deformity.

Additional indications include simple long bone fractures; severely comminuted spiral, large oblique and segmental fractures; polytrauma and multiple fractures; reconstruction, following tumor resection and grafting; supracondylar fractures; bone lengthening and shortening; fixation of fractures that occur in and between the proximal and distal third of the long bones being treated.

The OrthoPediatrics **Pediatric Nailing Platform | Femur** is for single use only.

When used in the European Union and the United Kingdom, the OrthoPediatrics **Pediatric Nailing Platform|Femur** is indicated for rotational osteotomy for excessive femoral anteversion and femoral fractures in pediatric patients. The System implants are for single use only. The System is indicated for patients 8 years or older; however, should the clinical situation dictate, and provided the recommended technique is followed, the use of this implant in younger patients is at the discretion of the surgeon.

SIZES AVAILABLE

The OrthPediatrics **Pediatric Nailing Platform | Femur** is available in child and adolescent configurations. Child nails come in 7mm, 8mm, and 9mm diameters. Adolescent nails come in 9mm, 10mm, 11mm, and 12mm diameters. Nail lengths range from 20cm to 48cm depending on the nail diameter and 50cm length nails upon special request.

Screw interlocking options are available both proximally and distally.

SYSTEM OVERVIEW

PREOPERATIVE PLANNING

Effective preoperative planning allows the surgeon to predict the impact of different interventions in order to perform the correction in the most accurate and safe manner. Optimal intramedullary nail fit, landmarking for entry point, entry angle, and assessment of alignment and rotation can be evaluated through preoperative radiographic analysis. Preoperative planning also allows the surgeon to have the appropriate implants available at the time of surgery.

The objectives of preoperative planning include:

- Determination of anticipated nail diameter and nail length.
- Establishment of appropriate anatomic landmarks, including the greater and lesser trochanters and physes.
- In the case of rotational osteotomies, determination of the extent of correction needed.

The overall objective of preoperative planning is to enable the surgeon to gather anatomic parameters which will allow accurate intra-operative placement of the implant.

NAIL SIZE SELECTION

Choosing the appropriate nail diameter and length are crucial to a successful surgical procedure. When selecting the diameter of the intramedullary nail to be used, it is not necessary to fill the entire intramedullary canal to achieve a tight isthmic fit with the nail.

Choosing the length of the nail can be done intra-operatively using the Nail Measuring Tool. After passing the 800mm Reaming Rod into the distal fragment, a direct measurement can be made with the Nail Measuring Tool.

Alternatively, use the OrthoPediatrics PediNail templates to estimate nail length and diameter. To estimate nail diameter, place the template on the AP or lateral x-ray of the femur and measure the diameter of the medullary canal at the isthmus. Take into consideration the thickness of the cortex at the isthmus when determining nail diameter.

To estimate nail length, place the template on the AP x-ray of the uninjured femur and otherwise normal femur and select the appropriate nail length based on patient anatomy.

NOTE: When selecting nail size, consider canal diameter, fracture pattern, patient anatomy and postoperative protocol.

Templates are available in 115% magnification in which the image is enlarged 15% to correspond to typical radiographic magnification; however, variations in magnification levels are common.

WARNING: The use of the **PNP|Femur system** is not recommended for fractures or osteotomies in which all of the distal screw holes cannot be fully contained in the distal fragment.

WARNING: The 7mm **PNP|Femur** nail is not recommended for patients weighing greater than 75kg.

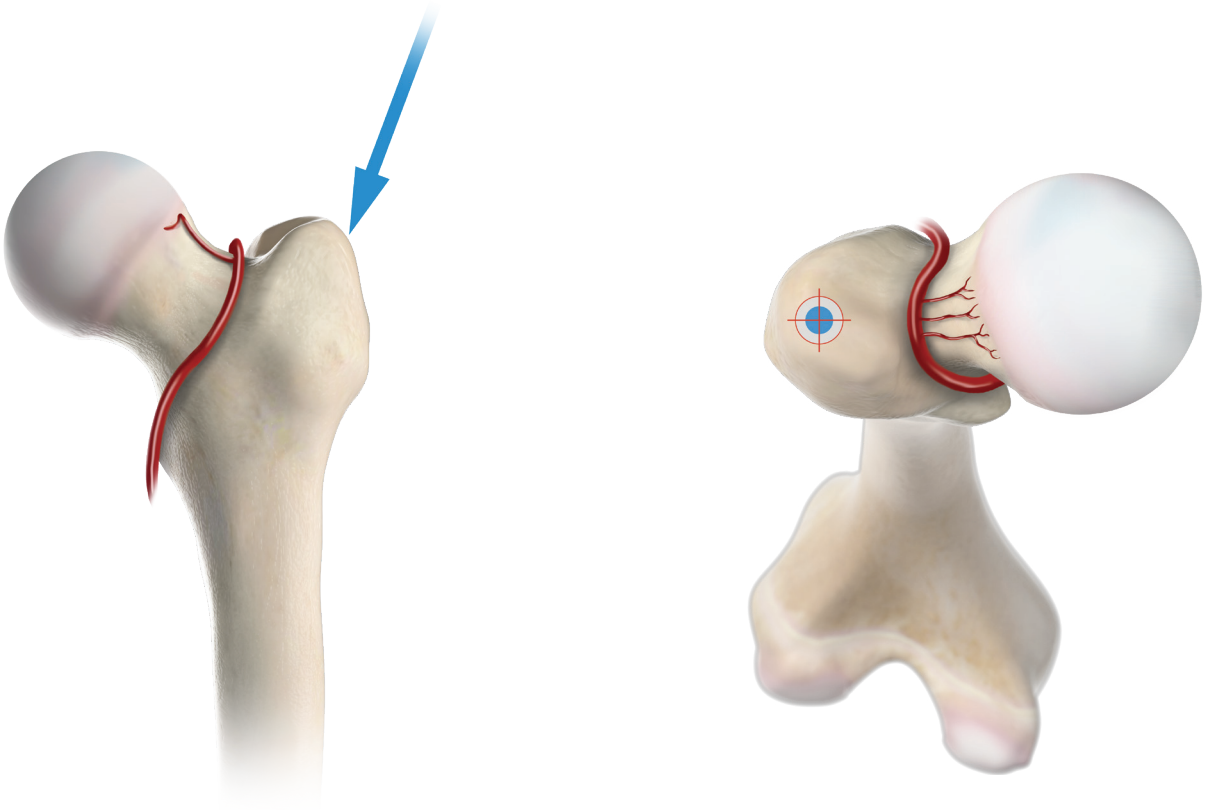


Figure 1: Entry point and entry angle.

Entry Point and Entry Angle

The Pediatric Nailing Platform | Femur intramedullary nail system is designed for use with a lateral trochanteric entry point for two reasons:

To avoid the piriformis fossa and subsequently the blood vessels of the medial circumflex artery supplying blood to the head of the femur, thus reducing the likelihood of iatrogenic femoral head avascular necrosis.

To avoid tethering the trochanteric growth plate, decreasing the risk of femoral neck narrowing and hip valgus.

The 10° proximal bend allows the entry point to be approximately 1 finger breadth lateral to the tip of the greater trochanter. The entry angle is measured from the entry point to a point inferior to the lesser trochanter (Figure 1).

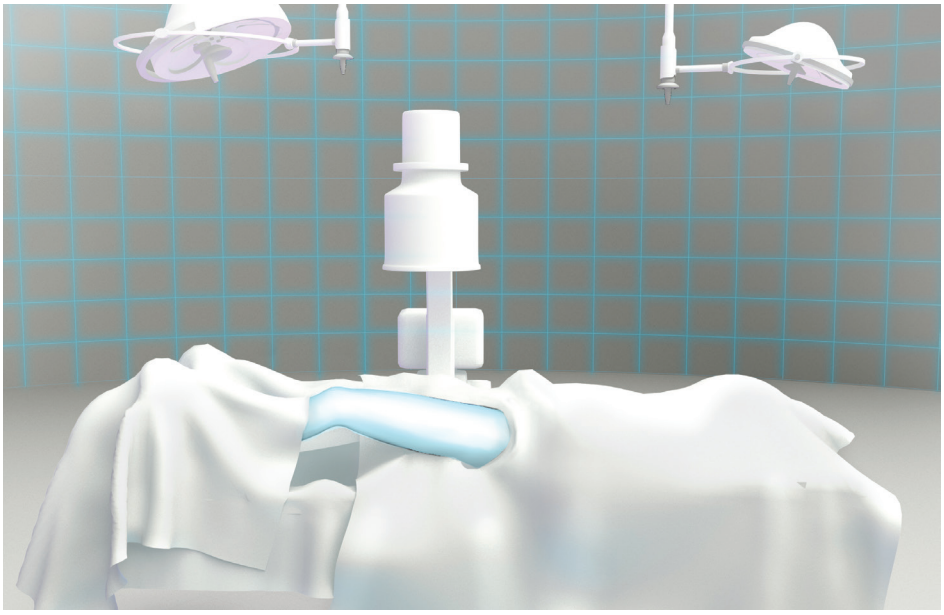


Figure 2: Patient positioning.

Patient Positioning

First, place the patient on a fracture table in the supine position.

Apply traction to the affected limb using a well-padded boot. Slightly externally rotate the limb to match the proximal fragment which tends to externally rotate slightly when the patient is positioned on the fracture table. Prep and drape the lower extremity using split sheets to allow circumferential access to the thigh. Cover the image intensifier with a sterile drape to visualize the hip and femur (Figure 2).

The proximal femur can be best visualized by arcing the image intensifier so the beam is directed from posteromedial to anterolateral. This allows the surgeon to see the externally rotated proximal femur in a non-rotated AP projection.

NOTE: Alternatively, the patient may be positioned supine on a radiolucent table. The limb (or both limbs in the case of bilateral procedures) can be prepared and draped free. This facilitates simultaneous irrigation and debridement of open femur fractures, bilateral rotation osteotomy, or fixation of an ipsilateral tibial fracture.

In order to bring the fracture out to length, an assistant may be required to apply manual traction.

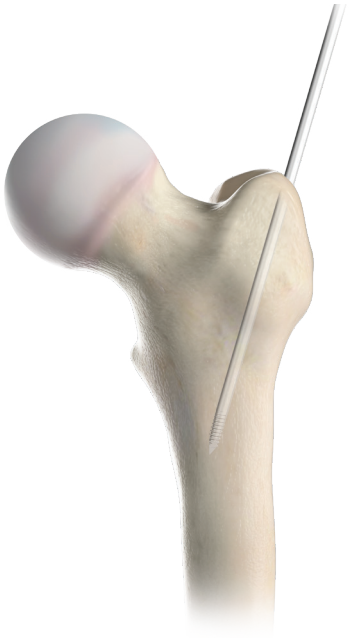


Figure 3: Insert Entry Pin into lateral aspect of greater trochanter.

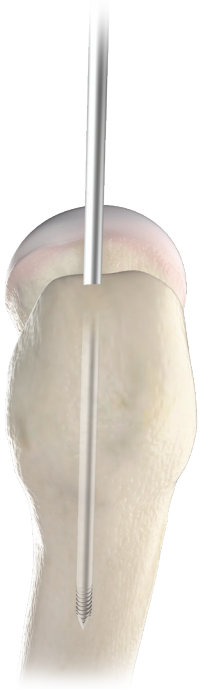


Figure 4: Lateral radiograph to ensure position in center of femoral canal.

Approach

Place the 3.2mm Entry Pin percutaneously through the lateral aspect of the greater trochanter at a point approximately halfway between the tip of the trochanter and the trochanteric physis.

Drive the 3.2mm Entry Pin under power with a drill through the trochanteric physis and into the medullary canal up to, but not through, the medial aspect of the proximal femur at an angle inferior to the lesser trochanter.

The 3.2mm Entry Pin should be 1.0-1.5cm distal to the lesser trochanter at an angle of 10° from the femoral shaft axis (Figure 3).

Check a lateral radiograph to insure that the 3.2mm Entry Pin is in the center of the femoral canal and is not inserted too shallow or too steep (Figure 4).

NOTE: Inspect pins and wires for any damage prior to use. Utilizing damaged instruments may adversely affect the outcome of the procedure.



Figure 5: Secondary Pin Guide (optional instrument).



Figure 6: Second Pin in desired position on AP and Lateral Planes.



Figure 7: Place Tissue Protector over the 3.2mm Entry Pin and into soft tissue.

Approach (cont.)

If the initial Entry Pin is not in the desired position in the AP and lateral planes, the optional Secondary Pin Guide can be used to place a second 3.2mm Entry Pin. Utilizing the fan-shaped slot, pass the Secondary Pin Guide over the initial wire. The Secondary Pin Guide can be angulated up to 10° relative to the initial pin. Place a second 3.2mm Entry Pin through one of the three holes adjacent to the slot. The central hole will position the starting point 5mm lateral to the initial wire. The two holes to either side of the central hole will position the starting point 5mm lateral and 5mm anterior/posterior, depending on the operative side (Figure 5). If the second wire is in an acceptable position, remove the initial wire and then remove the Secondary Pin Guide (Figure 6).

Create a 1.5cm incision proximal to the 3.2mm Entry Pin entry site, passing the scalpel adjacent to the guide wire, down to the trochanter.

Place the 10mm side of the Tissue Protector over the 3.2mm Entry Pin and into the soft tissue to protect the surrounding skin and soft tissue while using the opening reamer (Figure 7).

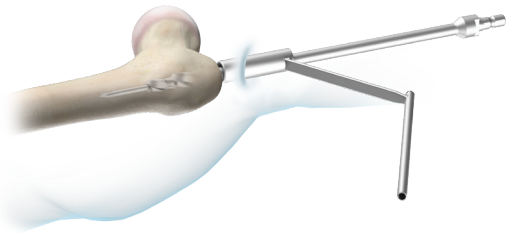


Figure 8: Advance 7.5mm/9.5mm Stepped Entry Reamer over 3.2mm Entry Pin.



Figure 9: AP radiograph to confirm placement in femoral canal and starting point.

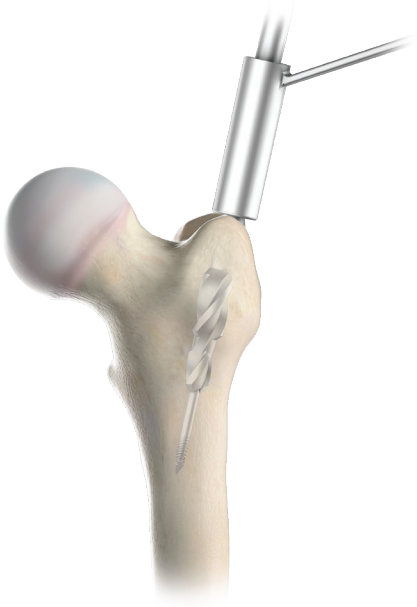


Figure 10: AP radiograph to check reamer.

Approach (cont.)

Advance the 7.5mm/9.5mm Stepped Entry Reamer over the 3.2mm Entry Pin through the trochanter into the femoral canal (Figures 8 - 10).

CAUTION: Never use the entry reamer without the Entry Pin.

CAUTION: Do not advance the Entry Pin or entry reamer past the medial femoral cortex.

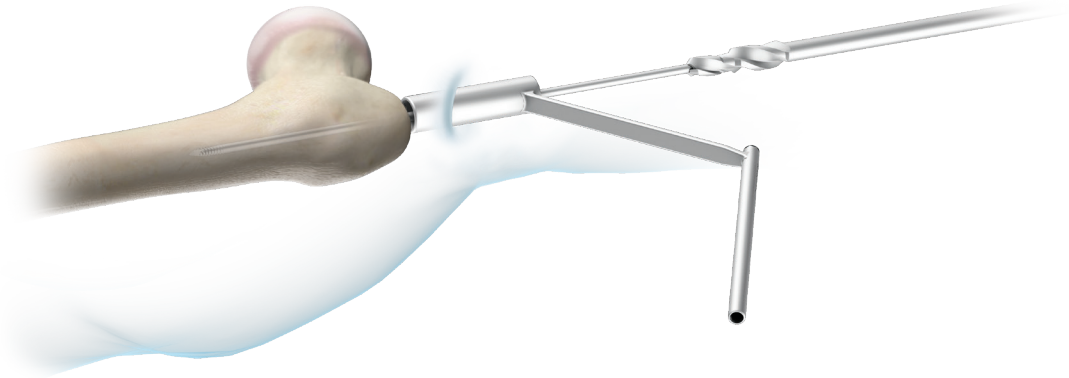


Figure 11: Withdraw 7.5mm/9.5mm Stepped Entry Reamer.

Approach (cont.)

Withdraw the 7.5mm/9.5mm Stepped Entry Reamer, leaving the 3.2mm Entry Pin in place in the proximal femur (Figure 11).

NOTE: If the 3.2mm Entry Pin appears to be lodged in the 7.5mm/9.5mm Stepped Entry Reamer, use the Guide Rod Obturator or Pusher, to ensure that the Pin remains in place upon removal of the reamer.

NOTE: Refer to Section 3: Reaming Technique (Reamer Use Guidelines).

With the 3.2mm Entry Pin and Tissue Protector still in place, place the desired reaming rod through the tissue protector and into the proximal femur. Confirm the reaming rod is in the proximal femur fluoroscopically and then withdraw the 3.2mm Entry Pin and Tissue Protector.



Figure 12: Assemble the Inserter.



Figure 13: Pass the Ball Tip Guide Wire through the knob-end of the inserter and tighten the knob.

Reaming Rod: Child Nails

The Child Nails will not allow passage of the 2.7/3.75mm x 800mm Ball Tipped Guide Wire through its cannulation. The 2.7/3.75mm x 800mm Ball Tipped Guide Wire will need to be exchanged for the 2.0mm x 800mm Smooth Guide Wire via the Exchange Tube prior to inserting the nail. Pass the wire down the femoral canal by hand or, if resistance is encountered, with the aid of the Inserter and Large Collet.

To assemble the Inserter, press and hold the silver button, load the Large Collet in the direction indicated by the arrow, release the button, and thread on the Knob (Figure 12). Pass the smooth end of the Ball Tipped Guide Wire through the knob end of the inserter and tighten the knob at the desired position along the wire (Figure 13). The wire is straight but a small bend can be created at the ball-tip end to aid in directing the wire, if needed.

NOTE: The Large Collet is for use with 2.7mm/3.75mm x 800mm Ball Tip Guide Wire. The Small Collet is for use with the 2.0mm x 800mm Smooth Guide Wire.

Reaming Rod: Adolescent Nails

The Adolescent Nails will allow passage of the 2.7/3.75mm x 800mm Ball Tipped Guide Wire through its cannulation. There is no need for a guide wire exchange. The same steps described above should be followed for placing the guide wire.

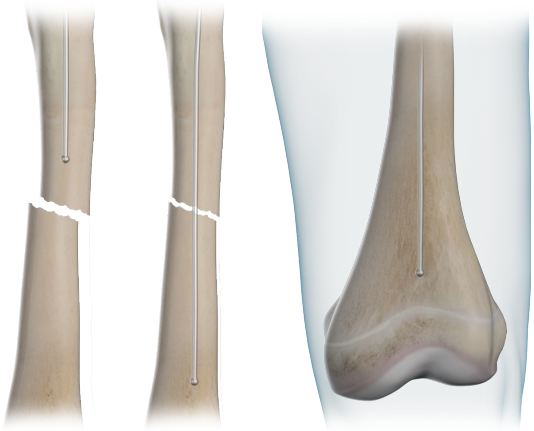


Figure 14: Pass the reaming rod down the femur, across the fracture, and to the distal metaphysis.

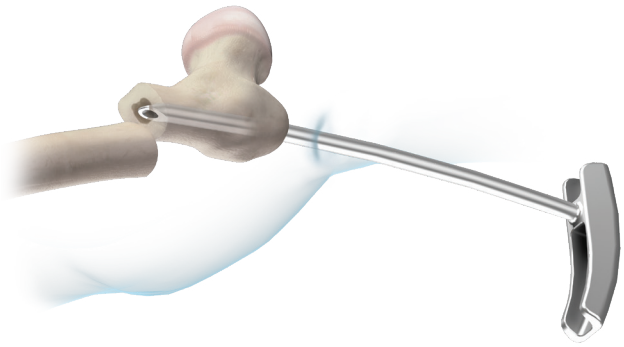


Figure 15: Use the Reduction Tool to control the proximal fragment in a subtrochanteric fracture.

Reaming Rod: Adolescent Nails (cont.)

Advance the reaming rod down the femur to the distal metaphysis. If treating a fracture, stop at the level of the fracture and use fluoroscopy to verify passage of the reaming rod across the fracture (Figure 14)

In subtrochanteric fractures the proximal fragment is often flexed, abducted, and externally rotated. In this setting, passing the reaming rod across the fracture can be challenging as the proximal fragment is difficult to control through traction and external manipulation. Use the Reduction Tool in the proximal fragment as a joystick to bring the fracture fragments into alignment, allowing passage of the reaming rod (Figure 15). Take care not to perforate the metaphysis with the Reduction Tool during manipulation.

NOTE: Verify placement using AP and ML fluoroscopy that reaming rod is in the distal fragment.

CAUTION: Do not advance reaming rod into physis or joint space.



Figure 16: Unfold the Nail Measurement Tool.



Figure 18: Read the measurement from the back of the wire.



Figure 17: Pass the Nail Measurement Tool over the reaming rod and advance to the surface of the greater trochanter.

Measuring

Prior to reaming, measure for the nail. When determining nail length, take care to accommodate for any distraction at the fracture site as well as the position of the guide wire in the distal femur to avoid penetration of the distal femoral physis by the nail.

Unfold the Nail Measurement Tool and pass it over the reaming rod. The metal ring will allow visualization of the instrument fluoroscopically to ensure it is contacting the greater trochanter (Figures 16 and 17).

Read the measurement from the back of the wire (Figure 18). The measurement obtained is a measure of the insertion depth of the guide wire. The surgeon should select a nail length using this measurement as a guide. Keep in mind that nails are often inserted 5mm below the surface of the greater trochanter.

NOTE: It is advisable to verify nail length using a second measurement method (i.e. two equal length reaming rods).

NOTE: The Nail Measurement Tool is calibrated for use with an 800mm wire. Using with a wire that is not 800mm will yield an inaccurate measurement. The XL Nails use the same reaming rod but different nail measurement tool.

Use the desired nail length to assess the nail diameters that could be used.

Nail Length	Nail Diameter
20cm - 38cm	7mm Child
24cm - 42cm	8mm Child
28cm - 42cm	9mm Child
28cm - 48cm*	9mm Adolescent
30cm - 48cm*	10mm Adolescent
30cm - 48cm*	11mm Adolescent
30cm - 48cm*	12mm Adolescent

* 50cm available upon special request



Figure 19: Create drill holes at the level of the osteotomy prior to distal reaming.

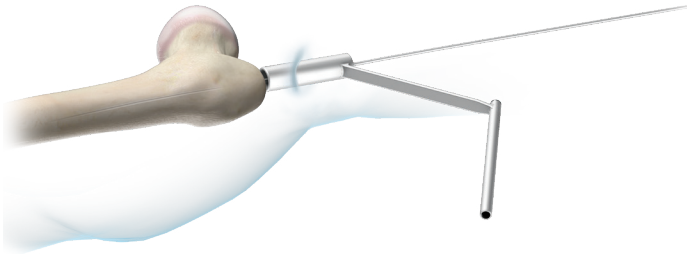


Figure 20: Protect skin at incision site with Soft Tissue Protector.

Measuring (cont.)

IF PERFORMING A ROTATION OSTEOTOMY

Withdraw the guide wire to the level of the osteotomy. Using the 3.8mm or 4.3mm Dill Bit and Osteotomy Drill Guide, make a number of drill holes at the site of the osteotomy through a small skin incision (Figure 19). Creating drill holes at the level of the osteotomy, by venting the canal, will reduce the likelihood of pulmonary emboli, the cause of which is fat and marrow displaced into the blood stream during intramedullary reaming. Do not complete the osteotomy at this time.

Once the drill holes have been created, pass the guide wire back down the femur and enlarge the canal through distal reaming.

Protect the skin at the incision site by sliding the 14mm side of the Tissue Protector over the guide wire and passing it down into the soft tissue (Figure 20).

Reaming Technique (Reamer Use Guidelines)

For most patients, utilize the flexible shaft with detachable side cutting reamer heads from 7.5mm to 14.0mm. The 14mm side of the tissue protector can be used with any size reamer. The 10mm side can only be used with reamers up to 10mm in size.

Under power, advance the reamer into the femoral canal. Keep advancing the reamer the entire length of the femur in a forward motion, up and down the entire length of the femur.

CAUTION:

ALWAYS FORWARD. Use power tool in the forward setting at all times.

ALWAYS ON. Do not stop the power tool.

Using fluoroscopy, confirm that the reamer has reached the distal end of the guide wire.

NOTE: Frequently clean the reamer flutes to prevent clogging.

If the reamer becomes stuck in the femoral canal, grasp the guide wire with a large needle holder or the Inserter and appropriate Collet and withdraw it 1 to 2cm while attempting to advance the reamer under power. If the reamer continues to be immovable, grasp the guide wire with a large needle holder or inserter and, using a mallet, tap on the inserter in a retrograde manner in order to remove the reamer and guide wire together.

CAUTION: Never reverse the reamer, as this could lead to reamer shaft failure.

Switch to the detachable side cutting reamers at size 7.5mm and continue reaming to desired diameter.

NOTE: It is not necessary to "fill" the canal or to continue reaming until "chatter" is noted. Appropriate selection of nail diameter is not dependent upon getting a tight fit in the isthmus of the femur.

NOTE: Be certain to exchange the 2.7mm Ball Tipped Reaming Rod with the 2.0mm Guide Insertion Rod if using a CHILD nail.

NOTE: Be certain to use the Guide Rod Obturator or Pusher when withdrawing the reamers to maintain the guide wire in the femoral canal.

CAUTION: If a small bend is created at the distal end of the 2.7mm Reaming Rod, do not ream past the bend as this may cause the reamer to bind and/or rupture.

WARNING: When performing a femoral osteotomy, to reduce the likelihood of pulmonary emboli, prepare the osteotomy prior to reaming or create vent holes in the femur.

CAUTION: For 6mm, 6.5mm, 7.0mm one piece front cutting reamers:

- Start with the 6mm reamer and go up in 0.5mm increments.
- Do not use in hard cortical bone.

NOTE:

- Recommended to over-ream 1.5mm to 2.0mm over desired implant diameter.
- If more distal reaming is needed, use reamer extender.
- Reamer extenders are available upon special request.

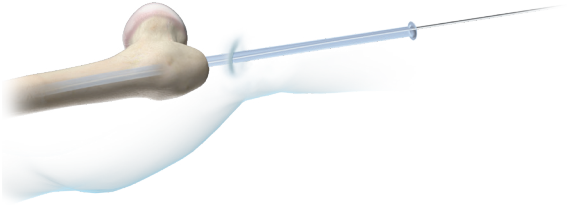


Figure 21: Place Exchange Tube over Ball Tipped Guide Wire.



Figure 23: Remove Ball Tipped Guide Wire and replace with Smooth Guide Wire.

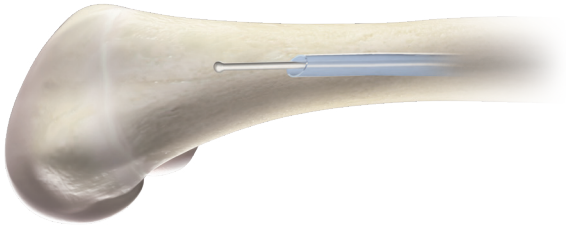


Figure 22: Verify placement of Exchange Tube.

Reaming Technique (Reamer Use Guidelines) (cont.)

For an Adolescent Nail, no guide wire exchange is necessary. If a Child nail is being used, the 2.7mm/3.75mm x 800mm Ball Tip Guide Wire must be exchanged for the 2.0mm Smooth Guide Wire prior to nail insertion. Place the Exchange Tube over the 2.7mm/3.75mm x 800mm Ball Tipped Reaming Rod and insert into the reamed femoral canal (Figure 21). Verify placement on radiograph (Figure 22).

Remove the 2.7mm /3.75mm x 800mm Ball Tipped Guide Wire and replace with the 2.0mm Smooth Guide Wire (Figures 23).

Remove the Exchange Tube.

NOTE: Removal of the 2.7mm/3.75mm x 800mm Ball Tipped Guide Wire without placement of the Exchange Tube or 2.0mm Guide Insertion Wire may result in loss of reduction.

CAUTION: If CHILD nail is implanted over 2.7mm/3.75mm x 800mm Ball Tipped Guide Wire, the guide wire will not be able to be removed.

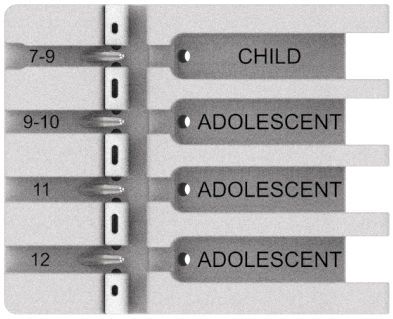


Figure 24: Retaining Alignment Fixture (RAF)



Figure 26: Properly loaded nail

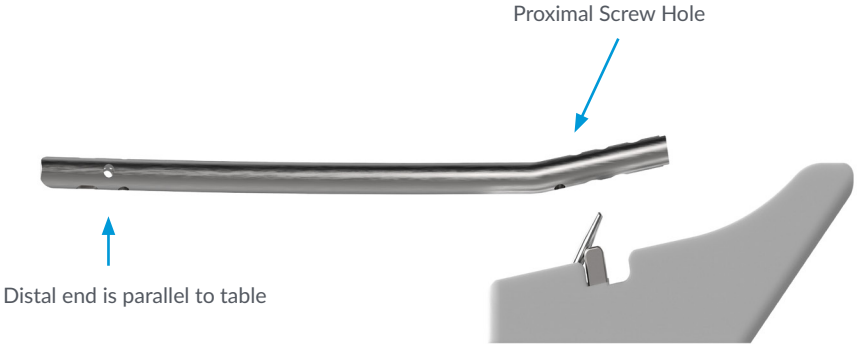


Figure 25: Load nail into RAF



Figure 27: Place guide into RAF, engage nail head and insert attachment bolt

Targeting Guide Nail Assembly

Attach the selected nail to the corresponding Targeting Device with the Attachment Bolt using the provided Retaining Alignment Fixture (RAF). The RAF is provided in a stand-alone, integrated tray. It should not be disassembled.

Targeting guides and Attachment Bolts are labeled “CHILD” and “ADOLESCENT”.

Select RAF slot based on chosen nail size.

Insert nail into fixture with the guide pin into the most proximal screw hole (descending oblique). Apply pressure to the nail head to fully seat in slot.

Place corresponding Targeting Guide into the RAF. Slide to engage with nail head.

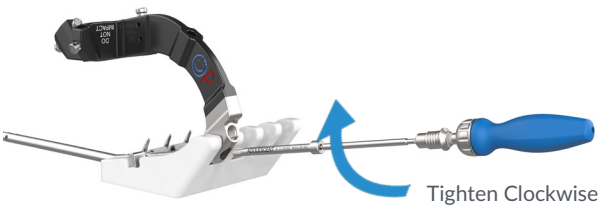


Figure 28: Insert Attachment Bolt and tighten turning clockwise

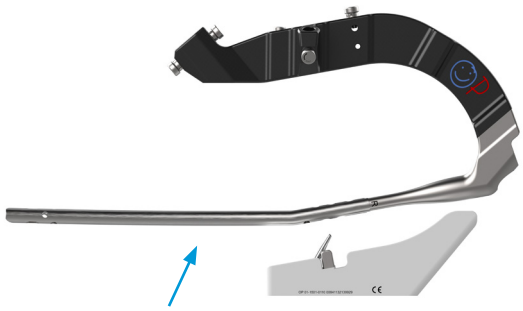


Figure 29: Remove assembled nail/targeting arm from RAF



Figure 30: Attach impactor to targeting device.



Targeting Guide Nail Assembly (cont.)

Insert Attachment Bolt through the Targeting Guide and into the nail. Utilize Ball Hex Driver to tighten bolt clockwise. If resistance is felt during the initial insertion of the bolt, STOP and reset.

Lift Targeting Guide/Nail Assembly out of the RAF, pulling inline with descending oblique screw hole.

CAUTION: Be certain that the Attachment Bolt remains tight throughout the impaction process. Failure to do so may lead to bolt breakage.

CAUTION: Attachment Bolt is a single-use device.

Nail Placement

Attach the Impactor to the threaded hole in the Targeting Guide after attaching the nail.



Figure 31: Confirm that nail is oriented correctly.

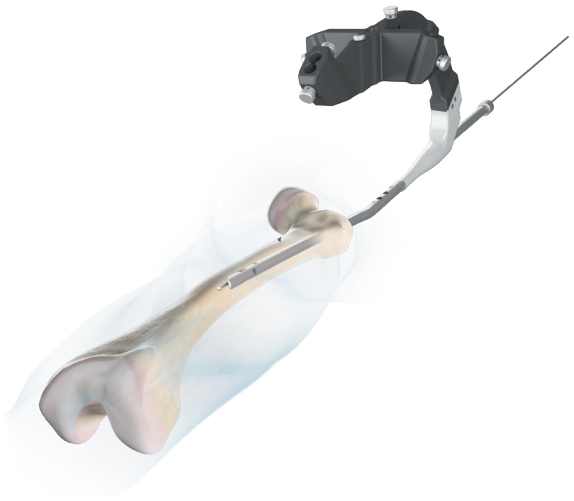


Figure 32: With the Targeting Guide pointing up, pass the nail into the proximal femur.

Nail Placement (cont.)

Prior to insertion of the nail, check alignment to ensure accurate targeting of the nail through the jig. Insert the Outer Screw Sleeve, the appropriate Inner Drill Sleeve, and the corresponding Trocar and make sure the Trocar passes through the interlocking holes in the nail (Figure 31).

Carefully pass the nail over the guide wire —2.7mm/3.75mm x 800mm Ball Tip Guide Wire for Adolescent Nails or the 2.0mm Smooth Guide Wire for Child Nails— and into the femoral canal to maintain location of the canal opening and to ease in insertion of the nail. Be sure that the nail slides freely over the guide wire to prevent advancement of the guide wire distally. Starting with the Targeting Guide pointing up towards the ceiling, pass the nail into the proximal femur and rotate the Guide laterally as the nail is inserted (Figure 33). Using controlled strikes with the mallet, drive the nail into the distal femur.

NOTE: Be certain that the impaction rod is fully seated with the flange on the impaction rod resting on the targeting guide. Maintain tightness and flange to targeting guide contact throughout the impaction process.

NOTE: If advancement of the nail is difficult, remove the nail and ream another 0.5mm. It is common to over ream the canal by 1.5-2.0mm. If additional reaming is necessary, be sure to use the appropriate guide wire.

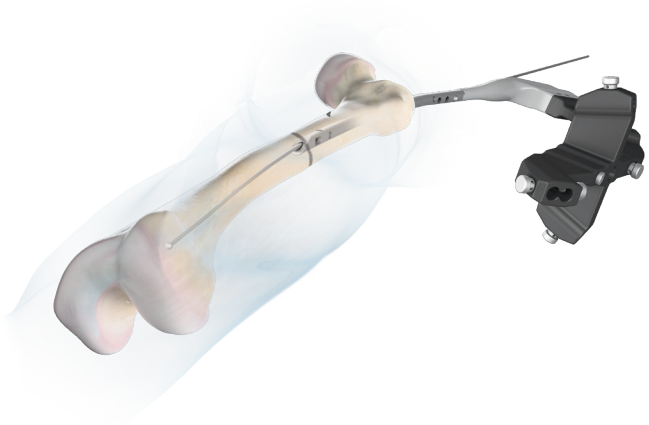


Figure 33: Advance the nail to the level of the osteotomy.

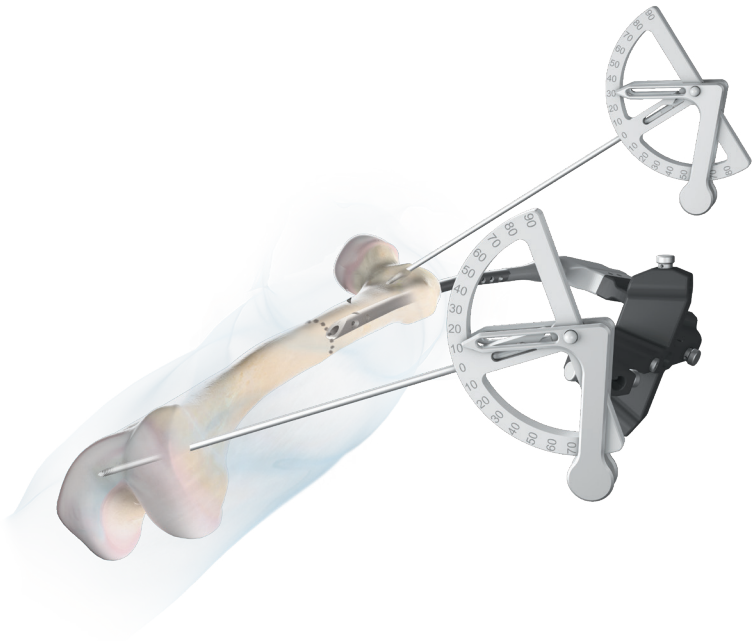


Figure 34: Place a 3.2mm Entry Pin above and below the osteotomy and measure the relative angle between them with the Derotation Dials. (optional instrument)

Nail Placement (cont.)

For rotational osteotomies, advance the nail to the site of the osteotomy (Figure 34). Place a 3.2mm Entry Pin across the femoral condyles and a second 3.2mm Entry Pin into the proximal femur taking care to avoid the nail. Attach the optional Derotation Dial to each pin to determine the initial relative angle between the pins prior to completing the osteotomy (Figure 34). Once the angles of the pins have been determined, remove the Derotational Dials, pull the guide wire back to the level of the osteotomy, and complete the osteotomy. Immediately advance the guide wire across the osteotomy and down the canal and continue advancing the nail into the distal femur. Leave the 3.2mm Entry Pins in place.



Figure 35: The Derotation Dial can be attached to the Targeting Guide via the Derotation Dial Attachment Pin.



Figure 36: Use the AP Position Jig and AP Template to determine appropriate insertion depth of nail.

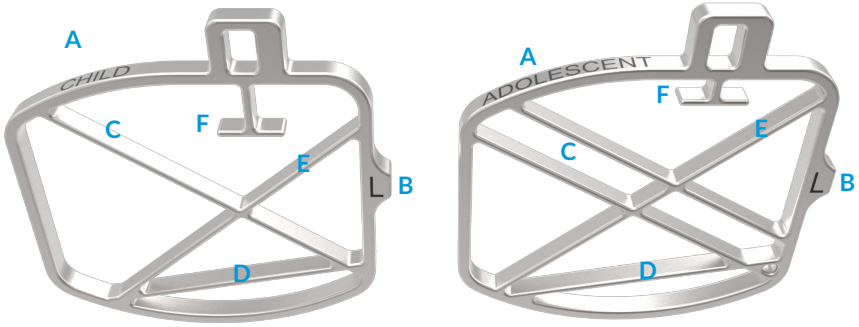


Figure 37: AP Templates: (A) Size; (B) Side; (C) Recon Screws; (D) Transverse Screw; (E) Descending Oblique Screw; (F) Nail Head. (optional instruments)

Nail Placement (cont.)

If planning to perform a rotational osteotomy with a recon screw up the femoral neck, no pre-osteotomy angular measurement is needed. Instead, the optional Derotation Dial can be attached to the Targeting Guide via the optional Derotation Dial Attachment Pin (Figure 35). When the recon screw is placed in the center of the femoral neck, the dial will indicate the true version of the femoral neck compared to a 3.2mm Entry Pin placed across the femoral condyles.

Impact the nail to approximately 5mm below the level of the trochanter but proximal to the trochanteric physis. The optional AP Position Jig and corresponding AP Template can be used to determine correct insertion depth (Figure 36). AP Templates indicate the head of the nail as well as the position of all proximal locking screws, as seen in the AP plane (Figure 37).

After the nail is inserted to the appropriate depth, remove the 2.0mm Guide Insertion Wire.

NOTE: Failure to remove guide wire may result in instrumentation damage and metal debris.

NOTE: The AP Templates are labeled “Child” and “Adolescent”, Left and Right. Be sure to use the correct card in the correct orientation.

NOTE: Be sure the image intensifier is positioned directly over the template ensure an accurate assessment of nail insertion depth and screw trajectories.

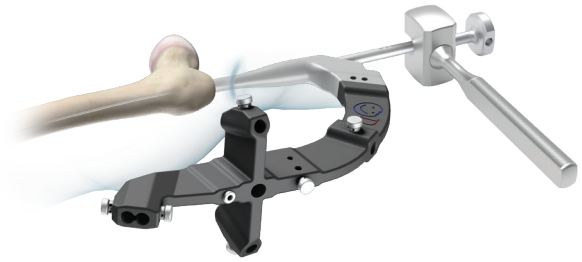


Figure 38: If inserted too deep, use Slotted Mallet to withdraw nail as needed.

CHILD Nail Proximal Locking	4.5mm Fully Threaded Screws	3.8mm Drill Sleeve (1 Green Band)	3.8mm Trocar (1 Green Band)	3.8mm Drill (1 Green Band)
	4.5mm Partially Threaded Screws	4.5mm Drill Sleeve (2 Green Bands)	4.5mm Trocar (2 Green Bands)	3.0/4.5mm Stepped Drill (2 Green Bands)
ADOLESCENT Nail Proximal Locking	5.0mm Fully Threaded Screws	4.3mm Drill Sleeve (1 Black Band)	4.3mm Trocar (1 Black Band)	4.3mm Drill (1 Black Band)
	5.0mm Partially Threaded Screws	5.0mm Drill Sleeve (2 Black Bands)	5.0mm Trocar (2 Black Bands)	3.5/5.0mm Stepped Drill (2 Black Bands)

Figure 39: Inner Drill Sleeve, Trocar, and Drill Bit combinations.

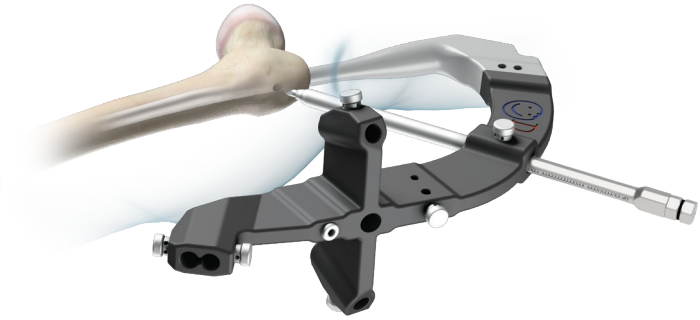


Figure 40: Advance sleeve assembly to the lateral cortex and secure in place with thumb screw.

Nail Placement (cont.)

If nail is inserted too deep, use the slot of the Slotted Mallet to withdraw the nail slightly. Use short strokes.

Once the nail is seated in its final position, confirm the attachment bolt remains securely tightened with ball hex driver.

Proximal Interlocking

Insert the Outer Screw Sleeve and appropriate Inner Drill Sleeve with corresponding Trocar through the desired hole in the Targeting Device and push down to the skin (Figure 39).

> **NOTE:** Do not apply excessive force to the targeting construct or targeting might be compromised.

Mark the skin with the Trocar and make a longitudinal incision. Bluntly dissect down to bone.

Make sure the Inner Drill Sleeve is advanced to the lateral cortex of the femur (Figure 40). Failure to do so will affect proximal screw measurement and insertion. Tighten the thumb screw on the Targeting Guide to lock the Outer Screw Sleeve in position. Do not over tighten the thumb screws.

Optional: Use the Trocar and light blows with a mallet to make a notch in the lateral cortex of the femur. This is done to ensure that the drill bit does not slip off the cortex (“skyve”) while drilling.

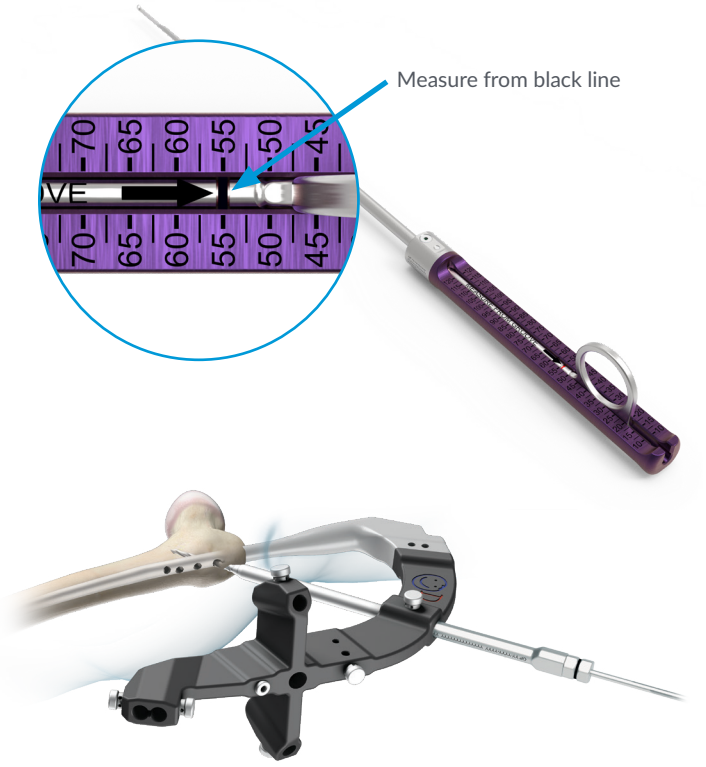


Figure 41: Insert Calibrated Drill Bit through the near cortex.

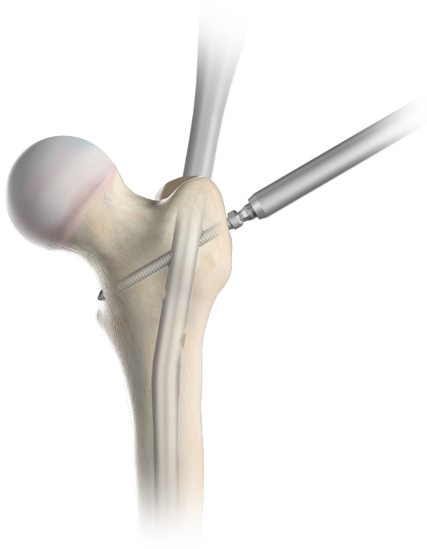


Figure 42: Verify screw position and length.

Proximal Interlocking (cont.)

Remove the Trocar and insert the appropriate Calibrated Drill Bit. Drill through the near cortex (Figure 41).

When the far cortex is reached, stop and measure from the calibration on the drill bit or use proximal depth guage.

Two hook depth gauges are available in the PNP system. The depth gauge referenced in Figure 41 will pass through the targeting arm tubes while the other hook depth gauge in the PNP system (referenced in Figure 48) will not.

The scale of proximal depth gauge is intentionally loose within the outer sleeve to facilitate engagement of the far cortex.

Advance the Drill Bit through the far cortex. Detach the drill bit from the drill and leave in place while selecting the appropriate screw. The screw caddy is labeled with screw size/type as well as with application and drill size. Take care to select the correct screw from the caddy.

Remove the Drill Bit and Inner Drill Sleeve. Insert the screw through the Outer Screw Sleeve and into the bone. Tighten the screw and remove the outer drill sleeve.

Verify screw position and length on AP and lateral image intensification (Figure 42).

> **NOTE:** If it is necessary to re-engage the driver into the screw head, it is recommended that the Outer Screw Sleeve is reinserted into the Targeting Device first.

See page 34 for information regarding the various screw drivers available in this system.



Figure 43: Preparation of recon screw.

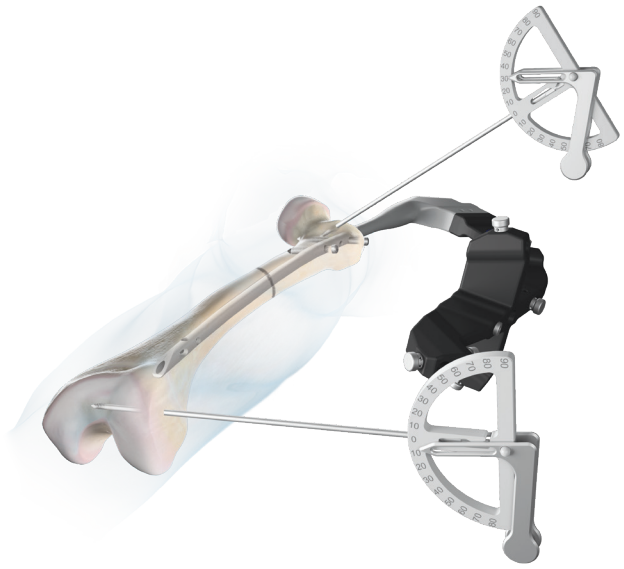


Figure 44: Measure relative angle between 3.2mm guide pins using the Derotation Dials.

Proximal Interlocking (cont.)

If a recon screw is to be used, place the Outer Screw Sleeve, appropriate Inner Drill Sleeve, and corresponding Trocar through the appropriate hole in the Targeting Guide and make a skin incision in line with the trajectory of the guide.

Advance the drill sleeves through the soft tissue, onto the bone. Be sure to notch the cortex with the trocar before drilling.

Drill with the appropriate calibrated stepped Drill Bit and measure. Insert the necessary length screw (Figure 43). The screw caddy is labeled with screw size/type as well as application and drill size. Take care to select the correct screw from the caddy.

NOTE: If placing two recon screws for adolescent nail simultaneously, the long retaining screw driver sleeve or proximal depth gauge may interfere with the second drill sleeve.

For rotational osteotomies after proximally locking the nail, re-attach the optional Derotation Dials to each 3.2mm Entry Pins. Rotate the distal femur to correct for the excessive anteversion. The difference between the initial relative angle and the final relative angle of the pins is the amount of rotation performed. For example, if the relative angle between the pins pre-osteotomy is 0° (pins parallel) and 25° post-osteotomy, then 25° of correction was achieved. Adjust the distal femur until the desired correction is reached.



Figure 45: Perfect circle distal interlocking.

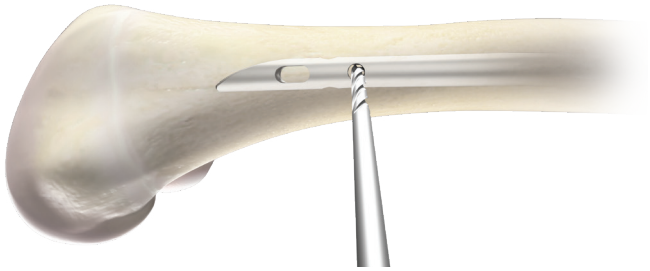


Figure 47: Position drill bit over the center of the hole.

CHILD Nail Distal Locking	7mm Nails	3.8mm Unicortical Peg	3.8mm Drill Bit
		4.0mm Fully Threaded Screw	3.2mm Drill Bit
	8mm Nails	4.5mm Fully Threaded Screws	3.8mm Drill Bit
	9mm Nails		
ADOLESCENT Nail Distal Locking	9mm Nails	4.5mm Fully Threaded Screws	3.8mm Drill Bit
	10mm Nails	5.0mm Fully Threaded Screws	4.3mm Drill Bit
	11mm Nails		
	12mm Nails		

Figure 46: Distal interlocking screw and drill bit combinations.

Distal Interlocking

Distal interlocking is carried out using the free hand technique.

Check rotation and length carefully prior to placing interlocking screws by examining the patient and examining the fracture site radiographically.

Place the image intensifier so that the interlocking hole makes a perfect circle in the center of the fluoroscopy monitor screen (Figure 45).

Make an incision over the center of the hole on either the anterior or lateral distal thigh depending on which interlocking hole is to be used. Select the appropriate drill bit for the nail implanted (Figure 46). Dissect bluntly through the soft tissue down to bone and position the drill bit over the center of the hole (Figure 47). If dynamization is desired, place the drill bit at the bottom of the slot. Drill through both cortices and disconnect the drill bit from the drill. Check radiographically to ensure that the drill bit has passed through the nail.

WARNING: Distal interlocking with a single dynamic screw is not recommended for length-unstable fractures at any location or length-stable fractures/osteotomies within 3cm of the superior-most distal screw hole.

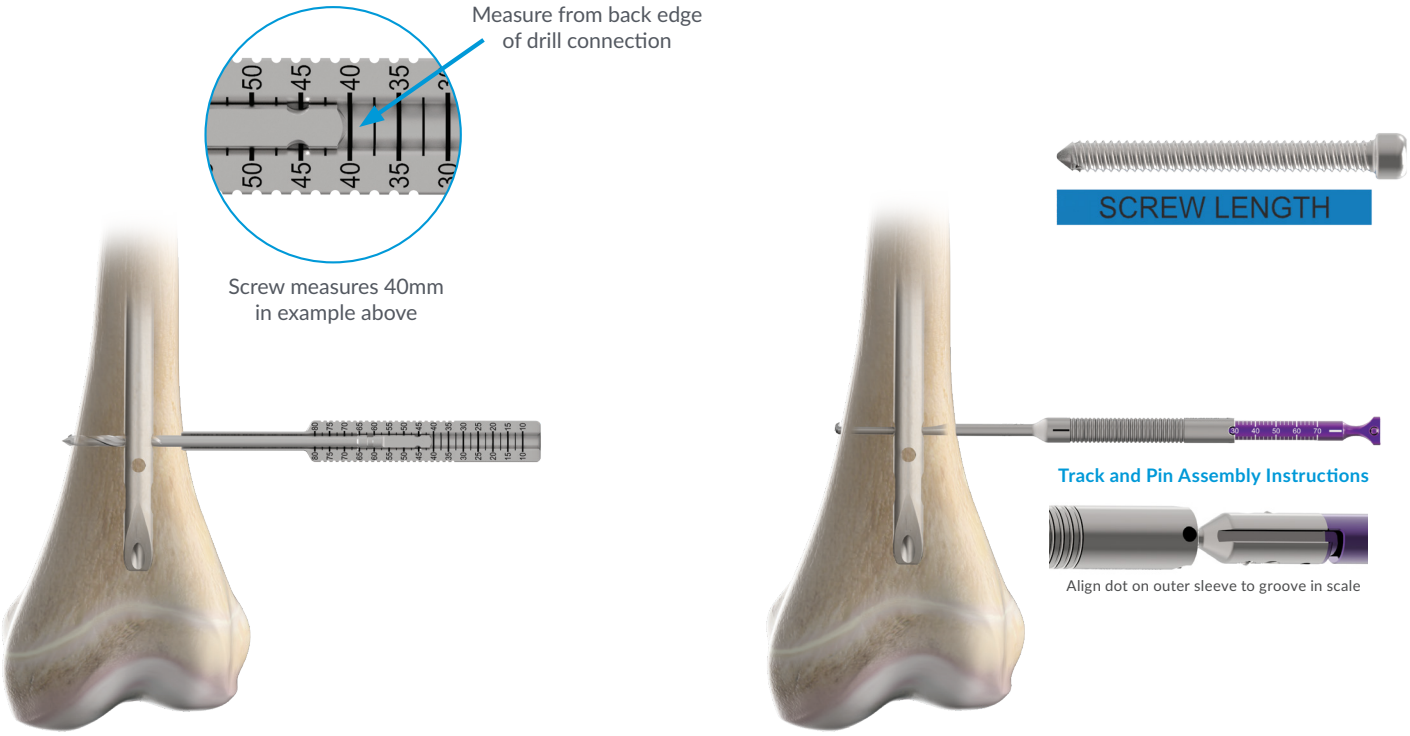


Figure 48: Measure for screw length with the sled or depth gauge.

Distal Interlocking (cont.)

Two options for distal measurement are provided. The Sled measures directly off the back edge of the drill bit. Alternatively, remove the drill bit from the hole and insert the depth gauge. Slide the hook of the depth gauge through the drilled hole and grab the far cortex with the hook. Slide outer sleeve against the near cortex and measure (Figure 48). Screw length is determined by working length and does not include the screw head.

Leaving the depth gauge in place, select the appropriate screw. The screw/end cap caddy is labeled with screw size/type as well as with application and drill size. Take care to select the correct screw from the caddy.



Figure 49: Check the screw for proper placement and length.

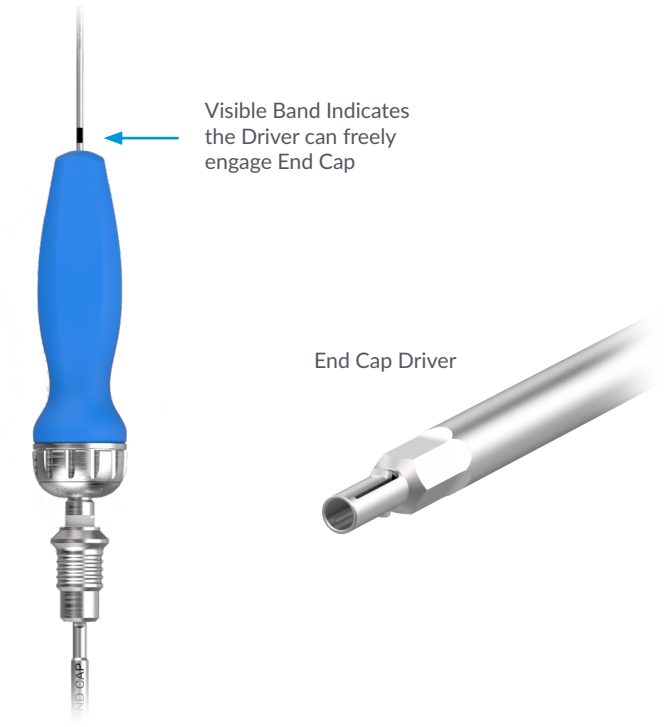


Figure 50: Place end cap driver, insert 2.0mm guide wire so black band is below proximal end of driver. This will engage locking mechanism.

Distal Interlocking (cont.)

When the appropriate screw is ready, remove the depth gauge and insert the screw. Check the screw for proper placement and length on AP and lateral image intensification. Verify radiographically (ML/AP) that screw is in distal locking hole of nail (Figure 49).

Repeat if two distal screws are desired.

Confirm final position of all implants—nail and screws—radiographically. After confirmation is complete, remove the Targeting Guide with the Ball Hex Driver

End Caps Option #1 - Non Retaining End Cap

If an End Cap is desired, reinsert the 3.2mm Entry Pin into the proximal portion of the nail. End Caps come in flush, +5, +10, +15, and +20mm lengths. They are also CHILD and ADOLESCENT nail specific. The Screw/End Cap Caddy is labeled with End Cap length/type. Chose an End Cap size so that the End Cap will sit at or just below the surface of the cortex. Take care to select the correct End Cap from the caddy.

Place the chosen End Cap onto the Cannulated T-Handle Hex Driver and pass it over the 3.2mm Entry Pin. End Caps feature a smooth projection below the threads to assist in orienting the End Cap to the nail. Screw the End Cap into the nail.

Option #2 - Retaining End Cap (if available)

If retaining end caps are available, assemble 2.0 guide wire, end cap and driver as shown in figure 50. Insert end cap and remove guide wire to disengage from driver once fully engaged in proximal head of nail. If black line is visible outside handle, the end cap can be disengaged. If it is sunk below the end of handle, the end cap is engaged onto wire.

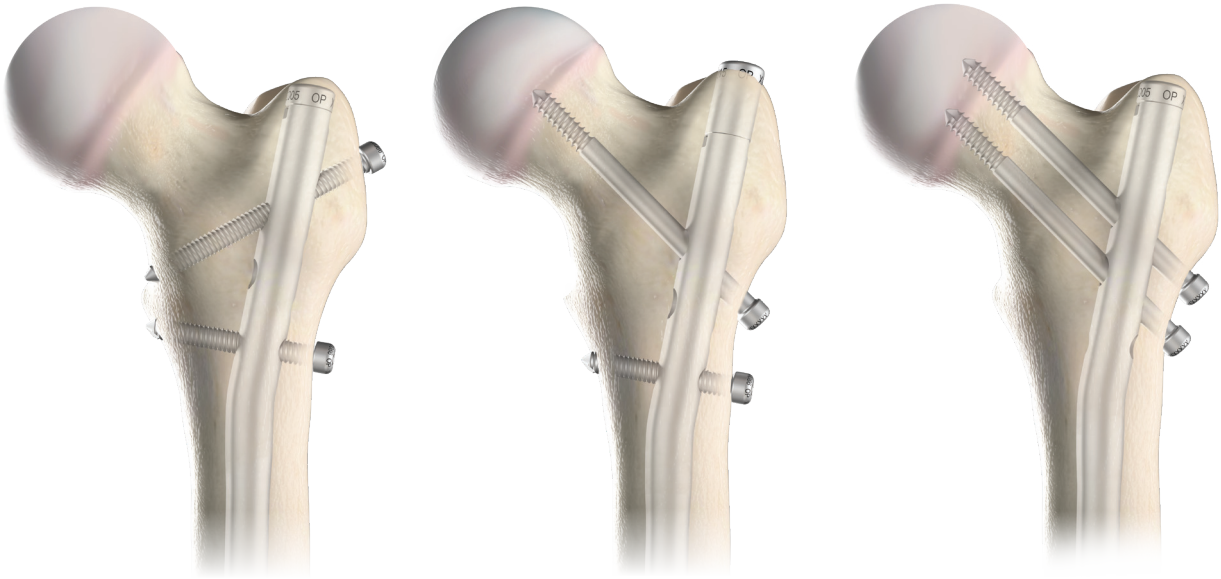


Figure 51: Possible ADOLESCENT Nail proximal locking configurations.

Closure and Post-Operative Care

Irrigate and close the surgical wounds in layers.

If adequate fixation has been achieved, no cast immobilization is required. The patient can be allowed toe-touch weight bearing or weight bearing as tolerated on crutches or a walker depending on the patient size and fracture stability.

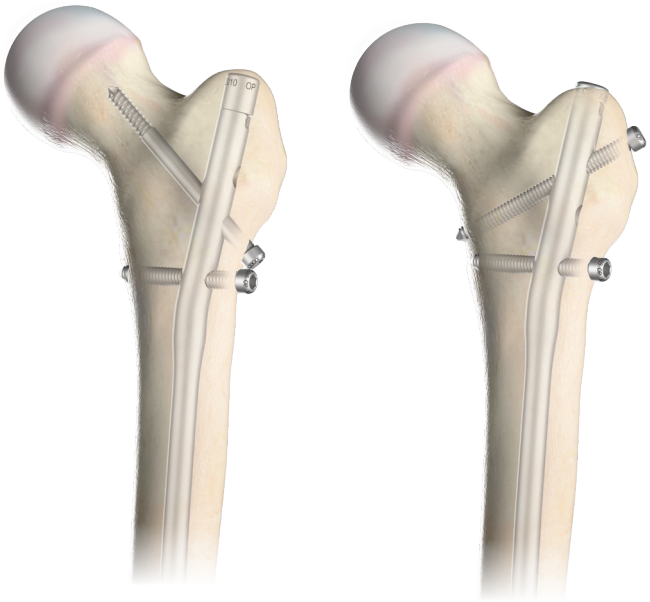


Figure 52: Possible CHILD Nail proximal locking configurations.

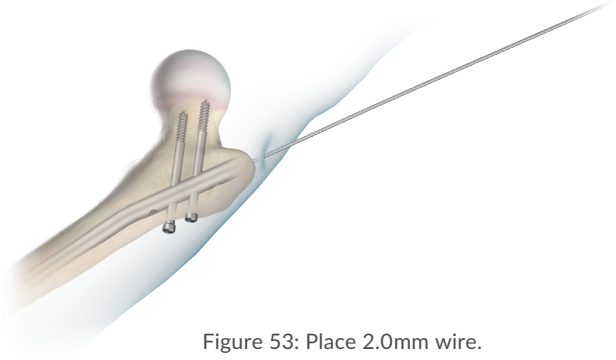


Figure 53: Place 2.0mm wire.

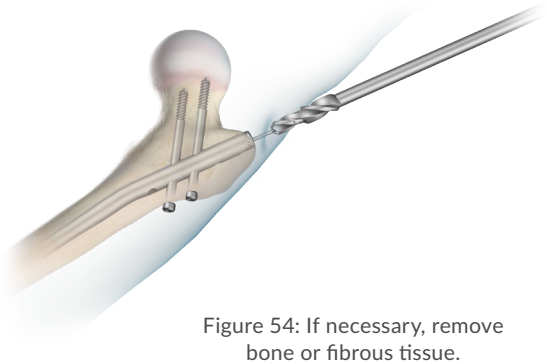


Figure 54: If necessary, remove bone or fibrous tissue.

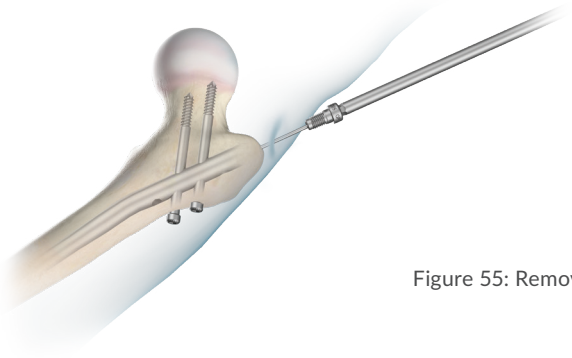


Figure 55: Remove end cap.

Nail Removal

NOTE: The conical extractors undergo significant stress when removing intramedullary nails. It is recommended that these items be used once and discarded. The Targeting Guide and Attachment Bolt are not intended for explantation.

Intramedullary nail removal, if desired, should be deferred, if possible, until after closure of the trochanteric physis (usually by age 13 to 14). For nail removal, position the patient supine on a radiolucent table with the hip and limb prepared and draped. Alternatively, the patient can be positioned in a lateral decubitus position to facilitate management of the soft tissue.

Make an incision through the scar created when inserting the nail. Bluntly dissect down to the greater trochanter. Place the 3.2mm Entry Pin (or any 2.0mm K-wire of adequate length), into the proximal end of the nail. Check position in both the AP and lateral planes (Figure 53).

If necessary, advance the 7.5mm/9.5mm Stepped Entry Reamer over the pin to the nail in order to remove bone or fibrous tissue over the proximal end of the nail (Figure 54).

WARNING: Do not allow reamer to contact metal implant.

If End Cap is in place, advance the 3.2mm Entry Pin through the hole in the End Cap and nail and pass the Cannulated T-Handle driver over the Guide Wire to the End Cap.

If retaining end cap is inserted, use 2.0mm wire and retaining end cap driver.

Remove the End Cap (Figure 55).

NOTE: Do not impact Cannulated T-handle driver.

01-1501-0128 (child) or 01-1503-0128 (adolescent)



01-1501-0078 (child) or 01-1503-0078 (adolescent)



Short vs. Long Conical Extractor



Cut away of threads inside each conical extractor

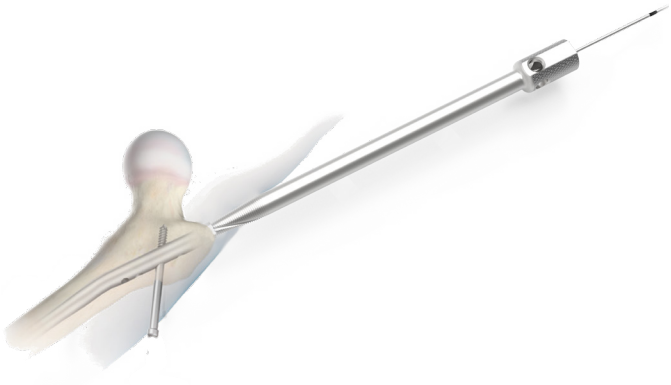


Figure 57: Pass Conical Extractor.

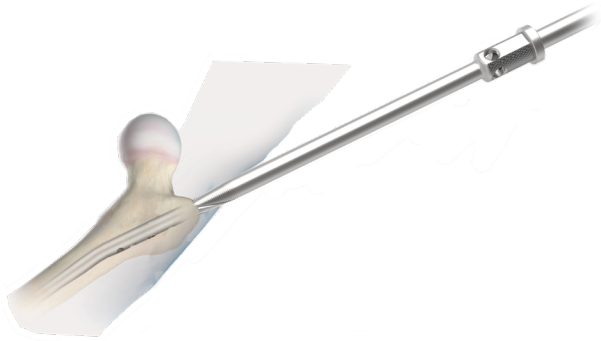



Figure 58: Remove locking screws and gently extract the nail.

Nail Removal (cont.)

Conical Extractors

NOTE: Two conical extractors are available which require different adaptors depending on which generation PNP|Femur instruments are available. When selecting conical extractor - adaptor combination, check to make sure the correct pair is selected.

Short conical extractor and fine threads on adaptor

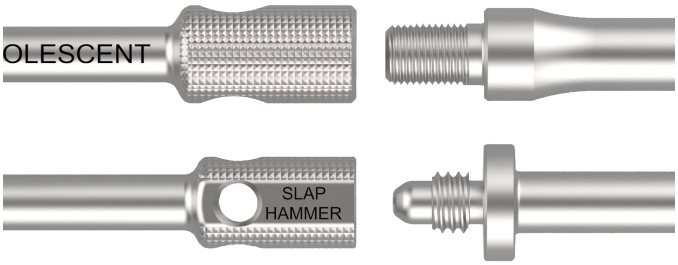

Long conical extractor and course threads on adaptor


Conical Extractor and Adaptor Compatibility


Conical Extractors feature a conical thread and reliefs to assist in clearing debris and ease of mating. All long Conical Cannulated Extractors use a 2.0mm wire. The short Child Conical Cannulated Extractors use a 2.0mm wire while the short Adolescent Conical Cannulated Extractor uses a 3.2mm wire.

Mate the appropriate conical extractor adaptor (CHILD or ADOLESCENT) with the nail (Figure 57).



Correct Conical Extractor and Adaptor Construct

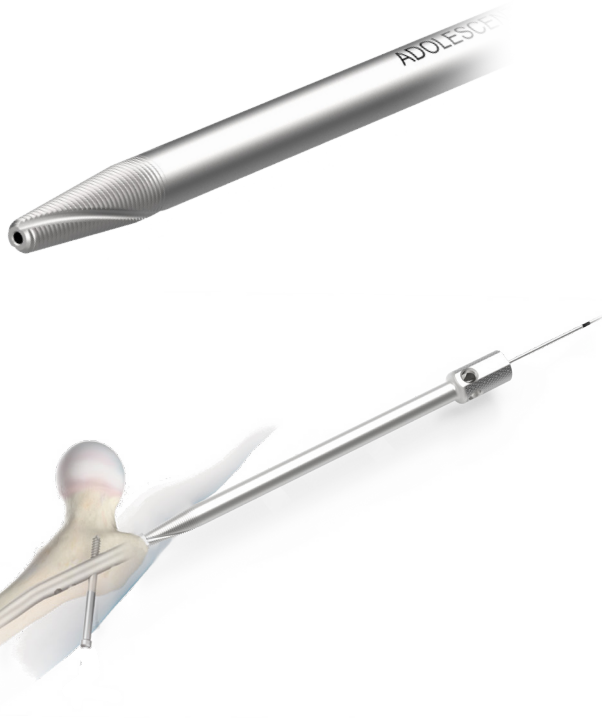

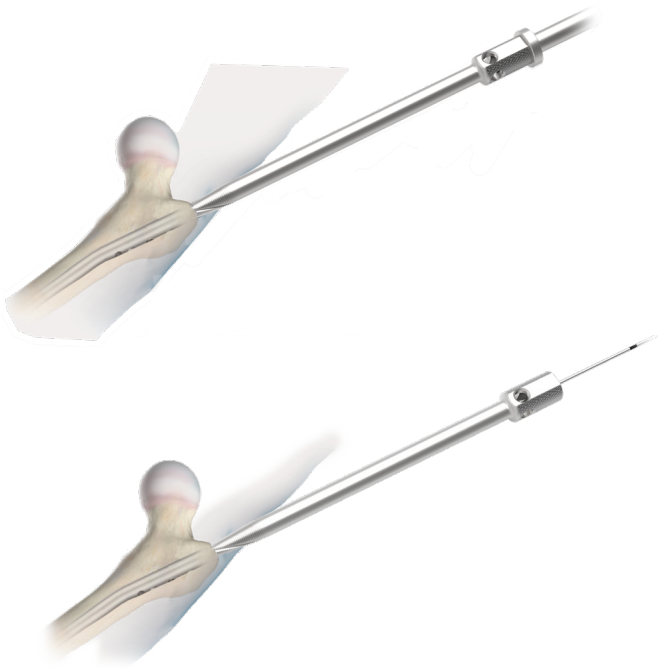

Extracting Nail

NOTE: The conical extractors undergo significant stress when removing intramedullary nails. It is recommended that these items be used once and discarded.

Insert Conical Cannulated Extractor over wire and mate to nail. Use the included tommy bar to ensure adaptor is tight.

NOTE: Ensure extraction adaptor is tight to avoid thread damage.

Remove all proximal and distal locking screws (see Screw Removal Section)

Remove guide wire, then attach appropriate Slap Hammer or Extraction Adaptor to the Conical Cannulated Extractor.

Extract with controlled blows.

NOTE: Avoid placing a bending moment on the adaptor.

NOTE: Excessive force in removal can cause bone damage.

	Thread
Pedinail Femur	1/4–20 UNC
PNP Femur Child	1/4–28 UNF
PNP Femur Adolescent	5/16–24 UNF

Closure

Irrigate and close the surgical wounds in layers.



Figure 60: 3.5mm Tapered Hex Driver.




Figure 61: Captured Screw Driver in disengaged position locked with screw.



Figure 62: Captured Screw Driver in engaged position capturing screw head.

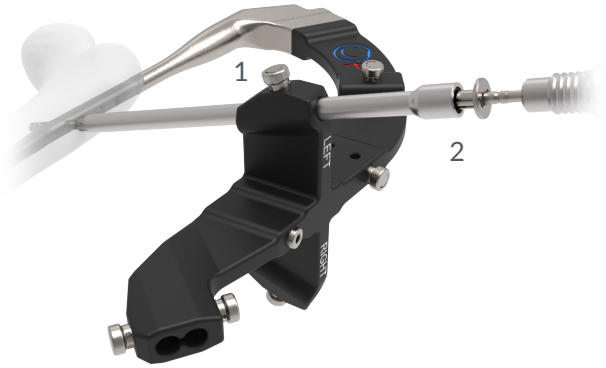


Figure 63: Loosen thumb screw (1) and then withdraw Outer Screw Sleeve against Captured Screw Driver Sleeve collar (2).

Screw Driver Options

Implantation Driver - Tapered Hex

The 3.5mm Tapered Hex Driver allows for easy retention of the screw on the driver with no moving parts (Figure 60). It is available in Long and Short lengths for proximal and distal interlocking, respectively.

Implantation Driver - Screw Capturing

The 3.5mm Captured Screw Driver is a two-piece driver - Shaft and Sleeve - that captures the head of the screw. The Sleeve has two positions, disengaged and engaged. In the disengaged position the 3.5mm hex is exposed for docking with the screw (Figure 61). Once the hex is docked with the screw, the Sleeve can be advanced to the engaged position where it can capture the screw head (Figure 62).

When using the long version through the Outer Screw Sleeve for proximal interlocking, the Outer Screw Sleeve prevents disengagement of the sleeve from the screw head. To release the screw, first unlock the Outer Screw Sleeve from the Targeting Guide by turning the thumb screw counterclockwise. Next, withdraw the Outer Screw Sleeve until it contacts the collar of the Captured Screw Driver Sleeve (Figure 63). Continue to pull the Outer Screw Sleeve against the collar until the screw head is released.

The Captured Screw Driver Shaft and Sleeve components reside disassembled in the instrument case.



Figure 64: Explant Driver in unlocked position docked with screw.



Figure 65: Screw backed out two turns with Sleeve in unlocked position.

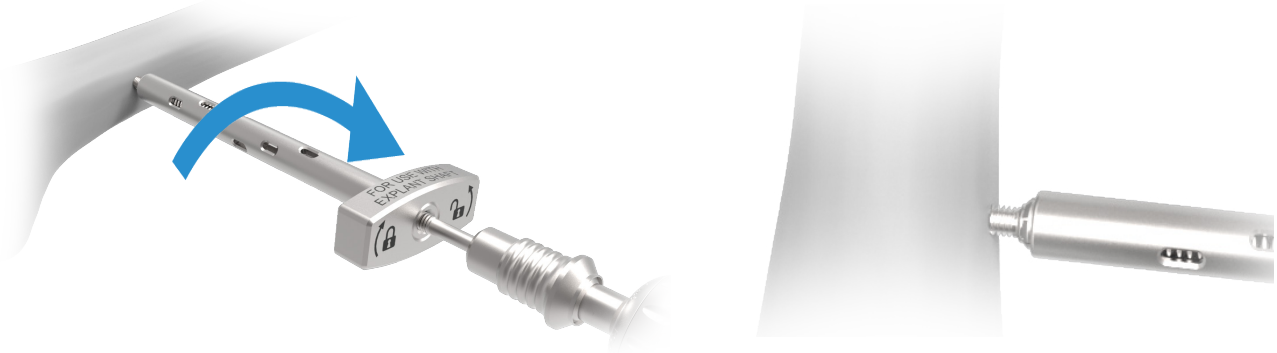


Figure 66: Explant Driver Sleeve in locked position.

Explantation Driver

The 3.5mm Explantation Driver is a two-piece driver - Shaft and Sleeve - that clamps onto the head of the screw. It is only available in Short length and will not function through the Targeting Guide. It is intended for screw removal.

The Sleeve has two positions, unlocked and locked. In the unlocked position the 3.5mm hex is exposed for docking with the screw. For screw removal, dock the 3.5mm hex with the screw (Figure 64). With the Sleeve in the unlocked position, back the screw out approximately two turns so that the screw head is completely clear of the cortex (Figure 65). Once the screw head is clear of the cortex, hold the driver handle stationary and turn the Sleeve clockwise to the locked position where it can clamp onto the screw head (Figure 66).

The Explant Driver Shaft and Sleeve components reside disassembled in the instrument case.

PRODUCT INFORMATION

CHILD LEFT FEMORAL NAILS

Description	Length (mm)	Quantity	Part Number
7mm x 20cm CHILD Left Nail	200	1	00-1501-0720
7mm x 22cm CHILD Left Nail	220	1	00-1501-0722
7mm x 24cm CHILD Left Nail	240	1	00-1501-0724
7mm x 26cm CHILD Left Nail	260	1	00-1501-0726
7mm x 28cm CHILD Left Nail	280	1	00-1501-0728
7mm x 30cm CHILD Left Nail	300	1	00-1501-0730
7mm x 32cm CHILD Left Nail	320	1	00-1501-0732
7mm x 34cm CHILD Left Nail	340	1	00-1501-0734
7mm x 36cm CHILD Left Nail	360	1	00-1501-0736
7mm x 38cm CHILD Left Nail	380	1	00-1501-0738
8mm x 24cm CHILD Left Nail	240	1	00-1501-0824
8mm x 26cm CHILD Left Nail	260	1	00-1501-0826
8mm x 28cm CHILD Left Nail	280	1	00-1501-0828
8mm x 30cm CHILD Left Nail	300	1	00-1501-0830
8mm x 32cm CHILD Left Nail	320	1	00-1501-0832
8mm x 34cm CHILD Left Nail	340	1	00-1501-0834
8mm x 36cm CHILD Left Nail	360	1	00-1501-0836
8mm x 38cm CHILD Left Nail	380	1	00-1501-0838
8mm x 40cm CHILD Left Nail	400	1	00-1501-0840
8mm x 42cm CHILD Left Nail	420	1	00-1501-0842
9mm x 28cm CHILD Left Nail	280	1	00-1501-0928
9mm x 30cm CHILD Left Nail	300	1	00-1501-0930
9mm x 32cm CHILD Left Nail	320	1	00-1501-0932
9mm x 34cm CHILD Left Nail	340	1	00-1501-0934
9mm x 36cm CHILD Left Nail	360	1	00-1501-0936
9mm x 38cm CHILD Left Nail	380	1	00-1501-0938
9mm x 40cm CHILD Left Nail	400	1	00-1501-0940
9mm x 42cm CHILD Left Nail	420	1	00-1501-0942

CASE & TRAY

Description	Quantity	Part Number
PEDIATRIC NAILING PLATFORM CHILD LEFT NAILS CASE AND LID	1	01-1501-0054

CHILD RIGHT FEMORAL NAILS

Description	Length (mm)	Quantity	Part Number
7mm x 20cm CHILD Right Nail	200	1	00-1502-0720
7mm x 22cm CHILD Right Nail	220	1	00-1502-0722
7mm x 24cm CHILD Right Nail	240	1	00-1502-0724
7mm x 26cm CHILD Right Nail	260	1	00-1502-0726
7mm x 28cm CHILD Right Nail	280	1	00-1502-0728
7mm x 30cm CHILD Right Nail	300	1	00-1502-0730
7mm x 32cm CHILD Right Nail	320	1	00-1502-0732
7mm x 34cm CHILD Right Nail	340	1	00-1502-0734
7mm x 36cm CHILD Right Nail	360	1	00-1502-0736
7mm x 38cm CHILD Right Nail	380	1	00-1502-0738
8mm x 24cm CHILD Right Nail	240	1	00-1502-0824
8mm x 26cm CHILD Right Nail	260	1	00-1502-0826
8mm x 28cm CHILD Right Nail	280	1	00-1502-0828
8mm x 30cm CHILD Right Nail	300	1	00-1502-0830
8mm x 32cm CHILD Right Nail	320	1	00-1502-0832
8mm x 34cm CHILD Right Nail	340	1	00-1502-0834
8mm x 36cm CHILD Right Nail	360	1	00-1502-0836
8mm x 38cm CHILD Right Nail	380	1	00-1502-0838
8mm x 40cm CHILD Right Nail	400	1	00-1502-0840
8mm x 42cm CHILD Right Nail	420	1	00-1502-0842
9mm x 28cm CHILD Right Nail	280	1	00-1502-0928
9mm x 30cm CHILD Right Nail	300	1	00-1502-0930
9mm x 32cm CHILD Right Nail	320	1	00-1502-0932
9mm x 34cm CHILD Right Nail	340	1	00-1502-0934
9mm x 36cm CHILD Right Nail	360	1	00-1502-0936
9mm x 38cm CHILD Right Nail	380	1	00-1502-0938
9mm x 40cm CHILD Right Nail	400	1	00-1502-0940
9mm x 42cm CHILD Right Nail	420	1	00-1502-0942

CASE & TRAY

Description	Quantity	Part Number
PEDIATRIC NAILING PLATFORMCHILD RIGHT NAILS CASE AND LID	1	01-1502-0054

ADOLESCENT LEFT FEMORAL NAILS

Description	Length (mm)	Quantity	Part Number
9mm x 28cm ADOLESCENT Left Nail	280	1	00-1503-0928
9mm x 30cm ADOLESCENT Left Nail	300	1	00-1503-0930
9mm x 32cm ADOLESCENT Left Nail	320	1	00-1503-0932
9mm x 34cm ADOLESCENT Left Nail	340	1	00-1503-0934
9mm x 36cm ADOLESCENT Left Nail	360	1	00-1503-0936
9mm x 38cm ADOLESCENT Left Nail	380	1	00-1503-0938
9mm x 40cm ADOLESCENT Left Nail	400	1	00-1503-0940
9mm x 42cm ADOLESCENT Left Nail	420	1	00-1503-0942
9mm x 30cm ADOLESCENT Left Nail	300	1	00-1503-1030
9mm x 32cm ADOLESCENT Left Nail	320	1	00-1503-1032
9mm x 34cm ADOLESCENT Left Nail	340	1	00-1503-1034
9mm x 36cm ADOLESCENT Left Nail	360	1	00-1503-1036
9mm x 38cm ADOLESCENT Left Nail	380	1	00-1503-1038
9mm x 40cm ADOLESCENT Left Nail	400	1	00-1503-1040
9mm x 42cm ADOLESCENT Left Nail	420	1	00-1503-1042
9mm x 30cm ADOLESCENT Left Nail	300	1	00-1503-1130
9mm x 32cm ADOLESCENT Left Nail	320	1	00-1503-1132
9mm x 34cm ADOLESCENT Left Nail	340	1	00-1503-1134
9mm x 36cm ADOLESCENT Left Nail	360	1	00-1503-1136
9mm x 38cm ADOLESCENT Left Nail	380	1	00-1503-1138
9mm x 40cm ADOLESCENT Left Nail	400	1	00-1503-1140
9mm x 42cm ADOLESCENT Left Nail	420	1	00-1503-1142
9mm x 30cm ADOLESCENT Left Nail	300	1	00-1503-1230
9mm x 32cm ADOLESCENT Left Nail	320	1	00-1503-1232
9mm x 34cm ADOLESCENT Left Nail	340	1	00-1503-1234
9mm x 36cm ADOLESCENT Left Nail	360	1	00-1503-1236
9mm x 38cm ADOLESCENT Left Nail	380	1	00-1503-1238
9mm x 40cm ADOLESCENT Left Nail	400	1	00-1503-1240
9mm x 42cm ADOLESCENT Left Nail	420	1	00-1503-1242

CASE & TRAY

Description	Quantity	Part Number
PEDIATRIC NAILING PLATFORM ADOLESCENT LEFT NAILS CASE AND LID	1	01-1503-0054

ADOLESCENT RIGHT FEMORAL NAILS

Description	Length (mm)	Quantity	Part Number
9mm x 28cm ADOLESCENT Right Nail	280	1	00-1504-0928
9mm x 30cm ADOLESCENT Right Nail	300	1	00-1504-0930
9mm x 32cm ADOLESCENT Right Nail	320	1	00-1504-0932
9mm x 34cm ADOLESCENT Right Nail	340	1	00-1504-0934
9mm x 36cm ADOLESCENT Right Nail	360	1	00-1504-0936
9mm x 38cm ADOLESCENT Right Nail	380	1	00-1504-0938
9mm x 40cm ADOLESCENT Right Nail	400	1	00-1504-0940
9mm x 42cm ADOLESCENT Right Nail	420	1	00-1504-0942
10mm x 30cm ADOLESCENT Right Nail	300	1	00-1504-1030
10mm x 32cm ADOLESCENT Right Nail	320	1	00-1504-1032
10mm x 34cm ADOLESCENT Right Nail	340	1	00-1504-1034
10mm x 36cm ADOLESCENT Right Nail	360	1	00-1504-1036
10mm x 38cm ADOLESCENT Right Nail	380	1	00-1504-1038
10mm x 40cm ADOLESCENT Right Nail	400	1	00-1504-1040
10mm x 42cm ADOLESCENT Right Nail	420	1	00-1504-1042
11mm x 30cm ADOLESCENT Right Nail	300	1	00-1504-1130
11mm x 32cm ADOLESCENT Right Nail	320	1	00-1504-1132
11mm x 34cm ADOLESCENT Right Nail	340	1	00-1504-1134
11mm x 36cm ADOLESCENT Right Nail	360	1	00-1504-1136
11mm x 38cm ADOLESCENT Right Nail	380	1	00-1504-1138
11mm x 40cm ADOLESCENT Right Nail	400	1	00-1504-1140
11mm x 42cm ADOLESCENT Right Nail	420	1	00-1504-1142
12mm x 30cm ADOLESCENT Right Nail	300	1	00-1504-1230
12mm x 32cm ADOLESCENT Right Nail	320	1	00-1504-1232
12mm x 34cm ADOLESCENT Right Nail	340	1	00-1504-1234
12mm x 36cm ADOLESCENT Right Nail	360	1	00-1504-1236
12mm x 38cm ADOLESCENT Right Nail	380	1	00-1504-1238
12mm x 40cm ADOLESCENT Right Nail	400	1	00-1504-1240
12mm x 42cm ADOLESCENT Right Nail	420	1	00-1504-1242

CASE & TRAY

Description	Quantity	Part Number
PEDIATRIC NAILING PLATFORM ADOLESCENT RIGHT NAILS CASE AND LID	1	01-1504-0054
ADOLESCENT XL NAILS CASE	1	01-1503-0055
ADOLESCENT XL NAILS CASE LID	1	01-1504-0056

IM NAIL END CAPS (NON-RETAINING)

Description	Length (mm)	Quantity	Part Number
CHILD Nail End Cap, Flush	0	1	00-1501-2000
CHILD Nail End Cap, 5mm	5	1	00-1501-2005
CHILD Nail End Cap, 10mm	10	1	00-1501-2010
CHILD Nail End Cap, 15mm	15	1	00-1501-2015
CHILD Nail End Cap, 20mm	20	1	00-1501-2020
ADOLESCENT Nail End Cap, Flush	0	1	00-1503-2000
ADOLESCENT Nail End Cap, 5mm	5	1	00-1503-2005
ADOLESCENT Nail End Cap, 10mm	10	1	00-1503-2010
ADOLESCENT Nail End Cap, 15mm	15	1	00-1503-2015
ADOLESCENT Nail End Cap, 20mm	20	1	00-1503-2020

IM NAIL ENDS CAPS (RETAINING)

Description	Length (mm)	Quantity	Part Number
PNP Child Nail End Cap, 0mm, Retaining	0	1	00-1501-3000
PNP Child Nail End Cap, 5mm, Retaining	5	1	00-1501-3005
PNP Child Nail End Cap, 10mm, Retaining	10	1	00-1501-3010
PNP Child Nail End Cap, 15mm, Retaining	15	1	00-1501-3015
PNP Child Nail End Cap, 20mm, Retaining	20	1	00-1501-3020
PNP Adolescent Nail End Cap, 0mm, Retaining	0	1	00-1503-3000
PNP Adolescent Nail End Cap, 5mm, Retaining	5	1	00-1503-3005
PNP Adolescent Nail End Cap, 10mm, Retaining	10	1	00-1503-3010
PNP Adolescent Nail End Cap, 15mm, Retaining	15	1	00-1503-3015
PNP Adolescent Nail End Cap, 20mm, Retaining	20	1	00-1503-3020

SCREW/END CAP CADDY

Description	Quantity	Part Number
PEDIATRIC NAILING PLATFORM SCREW/END CAP CADDY with LID	1	01-1501-0050

INTERLOCKING SCREWS

Length, mm	Qty	3.8mm Unicortical Peg	4.0mm Fully Threaded Screw	4.5mm Fully Threaded Screw	4.5mm Partially Threaded Recon Screw	5.0mm Fully Threaded Screw	5.0mm Partially Threaded Recon Screw
15	2		00-1506-6015	00-1506-2015		00-1506-4015	
17.5	2		00-1506-6017	00-1506-2017		00-1506-4017	
20	2		00-1506-6020	00-1506-2020		00-1506-4020	
22.5	2		00-1506-6023	00-1506-2023		00-1506-4023	
25	2	00-1506-1025	00-1506-6025	00-1506-2025		00-1506-4025	
27.5	2	00-1506-1027	00-1506-6027	00-1506-2027		00-1506-4027	
30	2	00-1506-1030	00-1506-6030	00-1506-2030		00-1506-4030	
32.5	2	00-1506-1033	00-1506-6033	00-1506-2033		00-1506-4033	
35	2	00-1506-1035	00-1506-6035	00-1506-2035		00-1506-4035	
37.5	2	00-1506-1037	00-1506-6037	00-1506-2037		00-1506-4037	
40	2	00-1506-1040	00-1506-6040	00-1506-2040		00-1506-4040	
42.5	2	00-1506-1043	00-1506-6043	00-1506-2043		00-1506-4043	
45	2	00-1506-1045	00-1506-6045	00-1506-2045	00-1506-3045	00-1506-4045	00-1506-5045
47.5	2	00-1506-1047	00-1506-6047	00-1506-2047	00-1506-3047	00-1506-4047	00-1506-5047
50	2	00-1506-1050	00-1506-6050	00-1506-2050	00-1506-3050	00-1506-4050	00-1506-5050
52.5	2	00-1506-1053	00-1506-6053	00-1506-2053	00-1506-3053	00-1506-4053	00-1506-5053
55	2	00-1506-1055	00-1506-6055	00-1506-2055	00-1506-3055	00-1506-4055	00-1506-5055
57.5	2	00-1506-1057	00-1506-6057	00-1506-2057	00-1506-3057	00-1506-4057	00-1506-5057
60	2	00-1506-1060	00-1506-6060	00-1506-2060	00-1506-3060	00-1506-4060	00-1506-5060
62.5	2			00-1506-2063	00-1506-3063	00-1506-4063	00-1506-5063
65	2			00-1506-2065	00-1506-3065	00-1506-4065	00-1506-5065
67.5	2			00-1506-2067	00-1506-3067	00-1506-4067	00-1506-5067
70	2			00-1506-2070	00-1506-3070	00-1506-4070	00-1506-5070
75	2			00-1506-2075	00-1506-3075	00-1506-4075	00-1506-5075
80	2			00-1506-2080	00-1506-3080	00-1506-4080	00-1506-5080
85	2			00-1506-2085	00-1506-3085	00-1506-4085	00-1506-5085
90	2			00-1506-2090	00-1506-3090	00-1506-4090	00-1506-5090
95	2			00-1506-2095	00-1506-3095	00-1506-4095	00-1506-5095
100	2			00-1506-2100	00-1506-3100	00-1506-4100	00-1506-5100
105	2				00-1506-3105		00-1506-5105
110	2				00-1506-3110		00-1506-5110
115	2				00-1506-3115		00-1506-5115
120	2				00-1506-3120		00-1506-5120

INSTRUMENT CASE 1

Description	Part Number	Description	Part Number
3.8mm Drill Sleeve Obturator	01-1501-0033	Stepped Entry Reamer 7.5mm/9.5mm	01-1500-0001
4.5mm Drill Sleeve Obturator	01-1501-0034	Osteotomy Drill Guide	01-1501-0010
4.3mm Drill Sleeve Obturator	01-1503-0033	Exchange Tube	11-1500-005
5.0mm Drill Sleeve Obturator	01-1503-0034	Inserter Body	01-1001-1001
3.8mm Drill Bit, Short, AO	01-1501-0018	Inserter Knob, Solid	01-1001-1003
3.8mm Drill Bit, Calibrated, AO	01-1501-0019	Collet, Small	01-1501-0036
4.5mm Recon Screw Stepped Drill Bit, Calibrated, AO	01-1501-0020	Collet, Large	01-1501-0037
4.3mm Drill Bit, Short, AO	01-1503-0018	Nail Measurement Tool	01-1501-0013
4.3mm Drill Bit, Calibrated, AO	01-1503-0019	Pusher	01-1500-031
5.0mm Recon Screw Stepped Drill Bit, Calibrated, AO	01-1503-0020	Outer Screw Sleeve	01-1501-0015
Tapered Screw Driver, 3.5mm, AO, Short	01-1501-0023	Inner Drill Sleeve, 3.8mm Drill	01-1501-0016
Tapered Screw Driver, 3.5mm, AO, Long	01-1501-0040	Inner Drill Sleeve, 4.5mm Drill	01-1501-0017
Captured Screw Driver Shaft, 3.5mm, AO, Short	01-1501-0025	Inner Drill Sleeve, 4.3mm Drill	01-1503-0016
Captured Screw Driver Sleeve, Short	01-1501-0038	Inner Drill Sleeve, 5.0mm Drill	01-1503-0017
Captured Screw Driver Shaft, 3.5mm, AO, Long	01-1501-0039	PNP Distal Direct Measuring Device	01-1501-0056
Captured Screw Driver Sleeve, Long	01-1501-0041	PNP Proximal Depth Gage Inner	01-1501-0066
AO QC Ratcheting Handle	01-1030-001	PNP Proximal Depth Gage Outer	01-1501-0067
T-Handle Hex Driver, Cannulated	01-1501-0024	PNP 3.2mm Drill Bit Short	01-1501-0068
Ball Hex Driver	01-1500-9019	PNP Femur Long Reduction Tool	01-1501-0111
3.2mm Entry Pin	11-1500-001	PNP Nail Depth Gauge, Scale Assembly 10-100mm	01-9000-1501
Tissue Protector	01-1501-0009	PNP Nail Depth Gauge, Outer Sleeve Assembly 10-100mm	01-9000-1502

Pediatric Nailing Platform Instrument Case #1 with Lid	01-1501-0151
Updated Instrument Case 1 Base	01-1501-0051
Instrument Case Lid	01-1501-0523
Updated Instrument Case 1 Upper Tier Tray	01-1501-0524

INSTRUMENT CASE 2

Description	Part Number	Description	Part Number
Child Nail Attachment Bolt, Single Use	01-1501-0032	Explant Driver Shaft, 3.5mm, AO	01-1501-0027
Adolescent Nail Attachment Bolt, Single Use	01-1503-0032	Explant Driver Sleeve	01-1501-0042
Proximal Targeting Guide, Child Nail	01-1501-0002	Impactor, Solid	01-1501-0035
Proximal Targeting Guide, Adolescent Nail	01-1503-0002	PNP End Cap Retaining Driver	01-1501-0064
PNP Child Conical Cannulated Extractor - Slap Hammer	01-1501-0078	PNP Tommy Bar	01-1501-0085
PNP Adolescent Conical Cannulated Extractor - Slap Hammer	01-1503-0078	2.0 X 450mm Smooth Wire	01-1501-0086
Pedinail Slap Hammer	01-1500-9013	PNP Gen II Slotted Mallet	01-1501-0108

Pediatric Nailing Platform Instrument Case #2 with Lid	01-1501-0052
PNP Instrument Case 2	01-1501-0152
Updated Instrument Case 2 Upper Tier Tray	01-1501-0520
Instrument Case Lid	01-1501-0523

IM REAMER CASE


Description	Part Number	Description	Part Number
6.0mm One Piece Flexible Reamer	01-1501-0060	10.0mm Modular Reamer Head	01-1500-100
6.5mm One Piece Flexible Reamer	01-1501-0065	10.5mm Modular Reamer Head	01-1500-105
7.0mm One Piece Flexible Reamer	01-1501-0070	11.0mm Modular Reamer Head	01-1500-110
Flexible Reamer Shaft	01-1500-060	11.5mm Modular Reamer Head	01-1500-115
7.5mm Modular Reamer Head	01-1500-075	12.0mm Modular Reamer Head	01-1500-120
8.0mm Modular Reamer Head	01-1500-080	12.5mm Modular Reamer Head	01-1500-125
8.5mm Modular Reamer Head	01-1500-085	13.0mm Modular Reamer Head	01-1500-130
9.0mm Modular Reamer Head	01-1500-090	13.5mm Modular Reamer Head	01-1500-135
9.5mm Modular Reamer Head	01-1500-095	14.0mm Modular Reamer Head	01-1500-140

Pediatric Nailing Platform IM Reamer Case with Lid	01-1501-0053

OPTIONAL EQUIPMENT

Description	Part Number
Reamer Extender	01-1500-0061

RETAINING ALIGNMENT FIXTURE TRAY

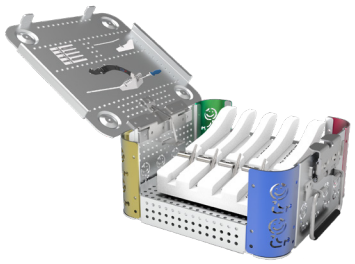

Description	Part Number
Retaining Alignment Fixture	01-1501-0100

MISCELLANEOUS INSTRUMENTS (NOT IN INSTRUMENT CASES)

Description	Part Number
2.7mm /3.75mm x 800mm Ball Tipped Guide Wire	01-1501-0800
2.0mm x 800mm Smooth Guide Wire	01-1501-0801

PNP XL NAILS (SPECIAL ORDER)

Description	Part Number
9mm x 440mm Adolescent Nail, Left	00-1503-0944
9mm x 460mm Adolescent Nail, Left	00-1503-0946
9mm x 480mm Adolescent Nail, Left	00-1503-0948
9mm x 440mm Adolescent Nail, Right	00-1504-0944
9mm x 460mm Adolescent Nail, Right	00-1504-0946
9mm x 480mm Adolescent Nail, Right	00-1504-0948
10mm x 440mm Adolescent Nail, Left	00-1503-1044
10mm x 460mm Adolescent Nail, Left	00-1503-1046
10mm x 480mm Adolescent Nail, Left	00-1503-1048
10mm x 440mm Adolescent Nail, Right	00-1504-1044
10mm x 460mm Adolescent Nail, Right	00-1504-1046
10mm x 480mm Adolescent Nail, Right	00-1504-1048
11mm x 440mm Adolescent Nail, Left	00-1503-1144
11mm x 460mm Adolescent Nail, Left	00-1503-1146
11mm x 480mm Adolescent Nail, Left	00-1503-1148
11mm x 440mm Adolescent Nail, Right	00-1504-1144
11mm x 460mm Adolescent Nail, Right	00-1504-1146
11mm x 480mm Adolescent Nail, Right	00-1504-1148
12mm x 440mm Adolescent Nail, Left	00-1503-1244
12mm x 460mm Adolescent Nail, Left	00-1503-1246
12mm x 480mm Adolescent Nail, Left	00-1503-1248
12mm x 440mm Adolescent Nail, Right	00-1504-1244
12mm x 460mm Adolescent Nail, Right	00-1504-1246
12mm x 480mm Adolescent Nail, Right	00-1504-1248
XL Nail Measurment Tool	01-1501-0087

IMPORTANT MEDICAL INFORMATION

Contra-Indications

Metallic bone fixation devices should not be used in patients with:

- active infections in or near the fixation site,
- a demonstrated sensitivity to metals,
- an inability to follow a post-operative regimen.

Warnings

- Federal (USA) law restricts this device to sale by or on the order of a physician.
- Before clinical use, the surgeon should thoroughly understand all aspects of the surgical procedure and the limitations of the instrumentation. Pre-operative procedures, knowledge of applicable surgical techniques, good reduction of bone fragments, proper patient selection and correct placement of the implants are all equally important for the successful use of these products.
- The 7mm PNP|Femur nail is not recommended for patients weighing greater than 75kg.
- The use of the PNP|Femur system is not recommended for fractures or osteotomies in which all the distal screw holes cannot be fully contained in the distal fragment.
- Distal interlocking with a single dynamic screw is not recommended for length-unstable fractures at any location or length-stable fractures/osteotomies within 3cm of the superior-most distal screw hole.
- The PNP|Femur I System is not intended to support the patient's weight as excessive loads may cause the device to fail. Weight bearing will depend upon the fracture pattern and stability, patient compliance and other associated injuries. Progression of weight bearing should be at the discretion of the surgeon.
- Use extreme care in the handling and storage of implants and instruments. Cutting, bending or scratching the surface of metal components can significantly reduce the corrosion, strength, and fatigue resistance of the implant and instrument system.
- Repeat use of a surgical implant is strictly forbidden. Each implant used once must be disposed of properly. This is the same even where it appears to be intact. The device may have small faults or internal stresses that if the item is re-used may lead to fatigue failure.
- Mixing of implants from different suppliers is not recommended for reasons of metallurgy, mechanics and design. We decline all responsibility in the case of implants from different sources being mixed.
- Care should be taken not to cut through surgical gloves when handling any sharp-edged surgical instrument and to take into account the risk of infection if a cut appears.

Adverse Effects

The risks associated with this device are the same as with any metallic internal fixation device. These include, but are not limited to the following:

- Delayed or non-union that may lead to breakage of the implant
- Loss of fixation, attributable to non-union, osteoporosis, unstable comminuted fractures
- Bending, fracture, or migration of the implant
- Metal sensitivity, or allergic reaction to a foreign body
- Limb shortening, or decrease in bone density, due to compression of the fracture or bone resorption
- Pain, discomfort, or abnormal sensations due to the presence of the device
- Nerve damage due to surgical trauma
- Necrosis of bone
- Infection, both deep and superficial
- Death
- Vascular disorders including thrombophlebitis, pulmonary embolus, wound hematomas, avascular necrosis

These adverse effects include adverse effects that are important considerations for metallic internal fixation devices. These risks and general surgical risks should be explained to the patient prior to surgery.

MRI Safety Information

Please refer to the IFU for the MRI Safety Information

CAUTION: Federal law restricts this device to sale by or the order of a Physician.

CAUTION: Devices are supplied Non-Sterile. Clean and sterilize before use according to instructions.

CAUTION: Implants components are single-use. Do not reuse.

CAUTION: Only those instruments and implants contained within this system are recommended for use with this technique. Other instruments or implants used in combination or in place of those contained within this system is not recommended, unless otherwise stated.

NOTE: This technique has been provided by one of our medical advisors only as guidance and it is not intended to limit the methods used by trained and experienced surgeons.

This document is intended exclusively for experts in the field, i.e. physicians in particular, and expressly not for the information of laypersons.

The information on the products and/or procedures contained in this document in of general nature and does not represent medical advice or recommendations. Since this information does not constitute any diagnostic or therapeutic statement with regard to any individual medical case, individual examination and advising of the respective patient are absolutely necessary and are not replaced by this document in whole or in part.

The information contained in this document was gathered and compiled by medical experts and qualified OrthoPediatrics employees to the best of their knowledge. The greatest care was taken to ensure the accuracy and ease of the understanding of the information used and presented. OrthoPediatrics does not practice medicine and does not recommend any particular orthopedic implant or surgical technique for use on a specific patient. The surgeon is responsible for determining the appropriate device(s) and technique(s) for each individual patient.

OrthoPediatrics does not assume any liability, however, for the timeliness, accuracy, completeness or quality of the information and excludes any liability for tangible or intangible losses that may be caused by the use of this information.

Instructions For Use (IFU), cleaning instructions, and surgical techniques may be obtained by calling OrthoPediatrics® Customer Service at 574-268-6379. Read and understand indications, warnings, and adverse effects explained in IFU's prior to use.

OrthoPediatrics, ArmorLink, BandLoc Duo, Drive Rail, PediFlex, PediFoot, PediFrag, PediGraft, PediLoc, PediNail, PediPlates, PLEO, QuickPack, RESPONSE, Scwire, ShieldLoc, TorqLoc, PediPedal and the OP and Pedi logos are trademarks of OrthoPediatrics Corp. ApiFix and Orthex are trademarks of wholly-owned subsidiaries of OrthoPediatrics Corp.

OrthoPediatrics is a registered trademark in Brazil, S.Korea, and the U.S.A. PediLoc and PediPlates are registered trademarks in Chile and the U.S.A. The OP logo is a registered trademark in Colombia, European Union, Japan, and the U.S.A. The Pedi logo is a registered trademark in Argentina, Australia, Brazil, Chile, Colombia, European Union, Israel, Mexico, New Zealand, S.Korea, Taiwan, Turkey, and the U.S.A. ApiFix is a registered trademark in the U.S.A. ArmorLink is a registered trademark in the U.S.A. Scwire is a registered trademark in the U.S.A. ShieldLoc is a registered trademark in the U.S.A. TorqLoc is a registered trademark in the U.S.A. BandLoc Duo is a registered trademark in the U.S.A. Orthex is a registered trademark in the U.S.A. QuickPack is a registered trademark in the U.S.A.

OrthoPediatrics® Leading Innovation in Pediatric Orthopedics

CE 2797

CE Mark is valid only if also printed on the product label or device itself

2850 Frontier Drive | Warsaw, IN 46582
ph: 574.268.6379 or 877.268.6339 | **fax:** 574.268.6302
www.OrthoPediatrics.com

© 2022 ORTHOPEDIATRICS - ST-1501-01-04 REV A (October 2022).